

User Manual of Forced Convection Oven

Model : OF4 – P series
Manual No. : H12915L002 Version : 2.1

JEIOtech



⚠ WARNING

Please read this user manual carefully before using the product. Users should operate the product according to the operating instructions contained in this user manual. Users should be aware of cautions and warnings for your safety. Failure to follow these guidelines may result in serious injury or damage to your property.

Thank you for purchasing JEIOTECH's products.

JEIOTECH Co., Ltd. is committed to offer the customer service including product sales, technical service, and follow-up management. If you have any question about this user manual, please contact our sales department.

Quality Management System ISO 9001



ISO 9001 is a standard that defines the requirements for a Quality Management System (QMS). It ensures the suitability of implementation in order for suppliers to continuously provide products and services that meet the buyer's requirements. JEIOTECH Co., Ltd. obtained ISO 9001 certification from *Korean Foundation for Quality (KFQ)* since 1998 to provide better service. Under this certification system, we design, develop, produce and sell a wide range of products related to chemical engineering, environment and life. We also provide reliability testing equipment for electrical and electronic engineering. (Oven, incubator, constant temperature and humidity chamber, constant temperature water tank, low temperature circulation tank, heat exchanger, stirrer, etc.)

You can download the above image by visiting the following JEIOTECH site.

<http://www.jeitech.com>

Disclaimer

The material in this manual is for the users' information only. The products it describes are subject to change without prior notice, due to the manufacturer's continuous development program.

Copyright

No part of this manual may be reproduced or transmitted in any form or by any means, including photocopying, recording, or using information storage and retrieval systems, for any purpose other than the purchaser's own use, without the express written permission of JEIOTECH Co., Ltd.

©2025. All Rights Reserved. JEIOTECH Co., Ltd.

Third-party product names or brand names mentioned in this user manual may be the trademarks of their respective owners. JEIOTECH has no connection with those companies and we do not endorse or recommend them directly nor indirectly.

Contents

1.0	Safety.....	1
1.1	How to use and read this user's manual.....	2
1.1.1	Introduction.....	2
1.1.2	Summary of each Chapters.....	2
1.1.3	The Product Model of the Instrument.....	2
1.2	Responsibility.....	3
1.2.1	General Responsibility.....	3
1.2.2	User's Responsibility.....	3
1.2.3	Responsibility for maintenance.....	4
1.3	The Indications Used in this User Manual.....	5
1.3.1	Signal Word Panels.....	5
1.3.2	Safety Symbols.....	6
1.4	Instructions for safe use (required reading).....	8
1.4.1	Warnings.....	8
1.4.2	Caution.....	10
2.0	Functional Description.....	12
2.1	Introduction.....	13
2.2	Feature.....	13
2.2.1	Excellent Performance.....	13
2.2.2	Safety Enhancement.....	14
2.2.3	Improved Convenience.....	15
2.3	Structure.....	16
3.0	Installation.....	21
3.1	Components of the Instrument.....	22
3.2	Preparations before installation.....	23
3.2.1	Installation Condition.....	23
3.2.2	Installation Guidelines.....	24
3.2.3	Minimum required space for Installation location.....	25
3.2.4	How to install shelf and its support.....	26
3.2.5	Available Space.....	27
3.3	The labels attached to the instrument.....	28
3.4	Power Connection.....	29
3.5	Checklists before the Use.....	30
3.6	Stacking Set (Option).....	32
4.0	Operation.....	37

4.1	Controller Home Screen names and functions.....	38
4.2	Basic Mode.....	39
4.2.1	Start and Stop in the Basic Mode.....	41
4.2.2	Temperature Settings.....	42
4.2.3	Timer Settings and Control.....	43
4.2.4	Checking the Operation after Timer Setting.....	46
4.2.5	Setting the Temperature Ramping Rate.....	47
4.2.5.1	Change the temperature ramping rate value setting.....	47
4.2.5.2	How to use the temperature ramping rate function.....	47
4.2.6	Fan Speed Settings.....	49
4.2.7	Real Time Graph.....	52
4.2.8	USB Storage function.....	54
4.2.9	Instantaneous Outage Recovery Features.....	56
4.3	Program Mode.....	57
4.3.1	Operation and Stop in Program Mode.....	59
4.3.2	Setting Program Mode.....	60
4.3.3	Confirming the Information during the Operation.....	62
4.3.4	Program Operation Settings.....	63
4.3.4.1	Start Point Set.....	63
4.3.4.2	Setting the number of cycles and closure.....	65
4.3.4.3	Setting the Skip Retention Function.....	66
4.3.5	Tolerable Temperature and Tolerable Time.....	67
4.4	General Settings.....	70
4.4.1	Sound & Display.....	70
4.4.2	Clock.....	71
4.4.3	Language.....	72
4.4.4	Auto Run & Door Lock.....	73
4.4.5	Scheduler.....	75
4.4.6	Data.....	76
4.4.7	Event.....	78
4.4.8	Communication.....	79
4.5	System Settings.....	80
4.5.1	Temperature.....	81
4.5.2	Calibration.....	83
4.5.3	Auto Tuning.....	85
4.5.4	Alarm.....	87
4.5.5	Password.....	88
4.5.6	Factory Default.....	88
4.6	Safety Function.....	89
4.6.1	Safety Functions Related to Temperature.....	89

4.6.2	Safety Functions Related to Use	89
4.6.3	Alarm Display and Pop-up Notification Function	90
4.7	Over temperature limiter	91
5.0	Maintenance.....	92
5.1	Inspection Cycle.....	93
5.2	Cleaning the Instrument	95
5.2.1	Cleaning the interior part of the instrument	95
5.2.2	Cleaning exterior part of the instrument	95
5.2.3	Cleaning the accessories	96
5.3	Major maintenance checks	97
5.4	Movement and storage	98
6.0	Trouble Shooting	99
6.1	Trouble Shootings for abnormalities	100
6.2	Power Trouble Shootings for abnormalities	100
6.3	Error Handlings	101
6.4	Caution and warning alarms.....	102
6.4.1	Caution.....	102
6.4.2	Warning	102
7.0	Accessories	103
7.1	Types of Accessories.....	104
7.2	LC Green Box (Option).....	105
8.0	Dedicated Software.....	106
8.1	Installing the Monitoring Program	107
8.2	Connecting the software to the instrument.....	108
8.3	Communication Protocol.....	111
8.3.1	Overview of Communication Protocol	111
8.3.2	Data Format.....	111
8.3.3	Frame	111
8.3.4	Function Code	111
9.0	Appendix.....	112
9.1	Technical Specification	113
9.1.1	OF4-P Series.....	113
9.2	Disposal of Product	114
9.3	Warranty	114

9.3.1	Warranty period.....	114
9.3.2	Technical Service Contact Points.....	114
9.3.3	Certificate of Product Warranty	115

1.0 Safety

1.1 How to use and read this user's manual

1.1.1 Introduction

This user's manual is published for the force convection oven users. This manual contains the contents of the oven's installation, operation, and maintenance.

This manual can be used as a reference for the safe use of the instrument and its simple repair. Please do not repair the instrument without a technical support of our company. Never move the instrument without a help of technical expert of the laboratory devices and electronics.
Make sure to keep the user manual after use.

1.1.2 Summary of each Chapters

The chapter 1 provides safety information about the safe use of the instrument. Please make sure to read it before installation and operation.

The chapter 2 provides functional description about the introduction, features, and structure of the instrument.

The chapter 3 contains installation instructions for instrument confirmation and installation. Also, it describes preparation procedures before operation and installation.

The chapter 4 describes operation of the instrument including names and functions of the control panel and basic operating functions of the instrument.

The chapter 5 provides information of maintenance including cleaning, moving, and storing instrument.

The chapter 6 provides information troubleshooting for the event of abnormality that may occur during use of the instrument.

The chapter 7 lists accessories of the instrument and how to mount it.

The chapter 8 provides information about the dedicated S/W for monitoring the instrument including installation and its communication protocols.

The chapter 9 provides Appendix of the instrument including specifications, disposal, warranty, and technical support contacts.

1.1.3 The Product Model of the Instrument

This user manual is applicable to OF4-series instrument as listed below.

	Forced Convection Oven Series			
Product Model	OF4-03P(W)	OF4-05P(W)	OF4-10P(W)	OF4-15P(W)

1.2 Responsibility

You can maximize your safety while using the instrument only when you follow the instructions about the instrument operation and maintenance under general operation conditions.

All users must be fully aware of the safety rules described in this user manual and then operate the instrument in the hazard • warning • caution indications.

1.2.1 General Responsibility

Safety is the first priority in any case. The owner, users, and maintenance personnel of the instrument should be fully aware that safety is the most important part of their work.

If you are concerned about damage in terms of efficiency, please consider the impact of human and material damage on productivity occurred by safety insensitivity accidents. The most reliable way to increase efficiency and productivity is to establish effective safety programs and comply with safety rules.

In addition to maintaining and repairing the instrument regularly, please check the condition of the instrument every day to ensure the safety. Also, please be sure to be familiar with this user manual, which describes each function and safety guide for the instrument.

1.2.2 User's Responsibility

One of the most important users' responsibilities is to achieve efficient and productive experimentation.

However, those are not the only part of the users' responsibilities. Even though users should be aware of the performance and limitations of the instrument, sometimes the safety of the parties is forgettable due to their desire for efficiency. Safety rules or user manuals do not protect the users from injury while using the instrument.

Therefore, please always follow the safety guidelines to operate the instrument. Also, please report potential risk situations to your superiors and colleagues immediately.

Things to be aware of

- Do not operate or fix the instrument without taking proper training or fully familiarizing yourself with the user manual.
- Please check the power voltage, phase, and capacity indicated on the ID label, and then connect it correctly.
- Do not touch hands or parts of your body to any part of the instrument that may cause injury.
- When operating the instrument, be careful not to wear loose clothes or accessories. If you have long hair, please tie your hair or wear a hair cap for your safety.
- When the instrument is not in use, please turn off the power switch or unplug the power cord.
- If the instrument does not work normally or has been left unattended for a long time, please check all the settings before operating the instrument.
- If you need to move the instrument or use it after a long pause, make sure that the instrument is operating normally.
- Please stop using the instrument when it appears with the following status, please stop the operation immediately and report it to the middle manager.
 - Incomplete operation or condition
 - Short circuit
 - Inappropriate maintenance

1.2.3 Responsibility for maintenance

Proper maintenance is one of the most important part of your responsibilities for your safety. Maintenance personnel must be aware of the importance of the safety in order to maintain the instrument effectively.

Please cut off all the electrical supply when you need to remove, adjust, or replace parts of the instrument. Also, please mark the instrument with a warning sign, "working."

Please make sure that it is correctly connected to a grounded outlet that fits to this instruments' plug.

Do not operate the instrument until all workers clean the surroundings. Also, before the operation, please check if there is any abnormality of the functions.

1.3 The Indications Used in this User Manual

This user manual uses signal word panels, safety symbols, and non-safety symbols to prevent accidents or damage in advance. Before using the instrument, please be sure to be familiar with the following indications.

1.3.1 Signal Word Panels

Signal Word Panels are indications to inform users about accidents, damage, and risk levels. Safety signs consists of three individual components: safety warning signs, phrases, and specific colors complied with ANSIZ535.4-2007 and ISO 3864.

Safety Signs	Contents
	Indicates a hazardous situation which, if not avoided, will result in death, fatal injury, or property damage
	Indicates a hazardous situation which, if not avoided, could result in serious injury, or property damage
	Indicates a hazardous situation which, if not avoided, may result in minor injury or property damage.
	Notifies you careful actions that are not relevant to your injury

1.3.2 Safety Symbols

Safety symbols are visual symbols that nonverbally convey hazardous situations, risk prevention methods, consequences of hazardous situations, or combinations thereof. Please operate the product with caution to the following safety signs.

Mandatory			
	Read the manual.		Wear gloves.
	Wear a face mask.		Wear eye protection.
Prohibition			
	Avoid direct sunlight		Avoid high frequency noise
	Beware of corrosive fluids or cleaners		Avoid water
Warning			
	Safety alert symbol For general cautions		Beware of electrical shock
	Beware of flammable or fire.		Do not place combustible dust inside.
	Do not insert toxic chemical inside.		Do not take the device apart deliberately.

	Beware of hand crush or pinch.		Beware of foot crush.
	Beware of lifting hazards.		

1.3.3 Non-safety Symbols

The graphics below are used to convey important information about the use and characteristics of the instrument without further explanation.

Non-safety Symbols			
	Permissible ambient temperature		Altitude
	Relative humidity		Earth ground

1.4 Instructions for safe use (required reading)

This instrument has been manufactured reliably and stably only when the operators follow this user manual's instructions of installation, operation, and maintenance. Before you install or operate the instrument, please be aware of this user manual's instructions and safety precautions. If you have any questions or comments regarding to this user manual or the instrument, please contact our JEIOTECH sales department.

To prevent personal injury or damage to the instrument during the installation, operation, or maintenance, please be fully aware of the warnings and cautions shown below.

1.4.1 Warnings



1) Safety Labels

- Please be fully aware of all the safety labels.
- Do not remove or damage the attached safety labels.

2) Electricity and Power

- Before installing the instrument, you should check the power voltage, phase, and capacity displayed on the ID label and connect them correctly.
- Be sure to use a power supply with a grade 2 or higher grounding.
: If the power is not grounded or poorly grounded, it may cause a hazard risk to an operator or the instrument. Also, never ground in a gas or water pipe.
- Do not connect other devices at the same time with one outlet.
- Never use branch sockets or double taps.
: Over current can cause severe damage to cables, damage to instrument, and fire.
Do not operate the instrument when the power line is damaged.
- Improper power connections can cause damage to the instrument and serious personal injury or death.
Do not handle or touch the electrical cords or electrical components with wet hands.

3) Installation

- Avoid contact with toxic chemical to the inside of the instrument.
- Do NOT install the instrument where flammable gas may leak.
- Do NOT use or store combustible gas around the instrument.
- Do NOT operate the instrument where an explosion may be occurred by organic evaporation gas.
- Do NOT operate the instrument in presence of industrial harmful gas, exhaust gas, or metal dust.
- Do NOT install instrument around gas pipes or water pipes.
- Do NOT install instrument in places with high humidity or risk of leakage.
- Water and organic solvents in the control panel may cause electrical short circuits.
- Do NOT expose the instrument to direct heat sources or direct sunlight.
- Keep the ambient temperature of the instrument between 5 and 40°C and the relative humidity below 80%.
- Ensure that the height of the installation site is less than 2,000 meters above the sea level.

- Install the instrument on a solid and flat floor in a laboratory facilitated with safety equipment.
- The door opens up to 115° to the left, so sufficient space should be considered when installing the instrument.

4) Operating and Transfer Instructions

- Do NOT place explosive, flammable, combustible or oxidizable chemicals such as alcohol, benzene, gasoline, etc. on top of the instrument, store them or operate them inside the oven. There is a risk of fire, since the instrument is not a explosion proof structure.
- Do NOT place liquid containers on the instrument. Leakage of liquid may cause damage to the instrument.
- Do NOT allow moisture, organic solvents, dust, and corrosive gases into the operating parts and inside of the instrument.
- Do NOT use the instrument if it makes strange sounds, smells or smoke.
- Do NOT operate damaged or short-circuit equipment.
- Do NOT move the instrument when the power cord is connected or when the instrument is operating.

5) Repair and Modification

- Do NOT disassemble or modify the instrument at any time other than those described in this user manual.
- When handling electrical components inside the instrument, only qualified personnel should handle them.



Avoid direct sunlight.



Beware of corrosive materials.



Avoid water.



Beware of electrical shocks.



Beware of fire.



Avoid contact with toxic chemical to the inside of the instrument.




Do not disassemble deliberately.



Do not put flammable dust inside the device.

1.4.2 Caution

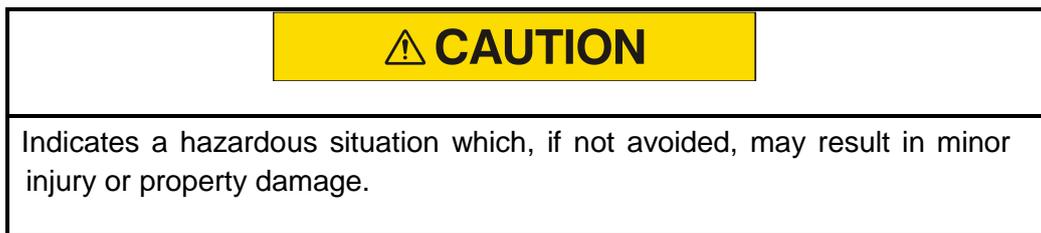

1) Power

- This instrument should use a grounded power cord
- When installing and using the product, always use a grounded power outlet.
- Plug the power tightly and correctly to prevent loosening from the outlet.
- Avoid heavy objects or the instrument to be placed on the power cord.
- When the instrument is not in use, be sure to turn off the main power switch before unplugging the power cord.

2) Installation

- Do NOT install the instrument near devices with strong and high frequency noise (high frequency welders, high frequency sewing machines, high-capacity SCR controls).
- Be aware that artificial heart pulses or magnetic data devices may be affected by magnetic bars of the oven.
- Do NOT install instruments adjacent to other experimental devices, electrical devices and power terminals.
- Do NOT install the instrument in unventilated corners. If the place is not sufficiently ventilated, there is a risk of damage to the instrument due to overheating by difficult heat dissipation.
- The device should be installed close to the outlet and should be easy to use.
- Maintain an appropriate clearance distance (typically at least 30 cm) from other instruments.

3) Machine Operation

- When initiating the instrument, the operator should check the machine continuously until it reaches to normal status.
- Wear gloves when handling samples to prevent burns since there may be residual heat during the operation or even when the power is off.
- Keep the instrument clean and make sure that there is no any foreign substances inside the chamber.
- Take a special care not to damage any accessories or systems inside the instrument.
- Be careful not to contact the main body with high concentrations of nitric acid, sulfuric acid, sodium hydroxide, or corrosive solvents such as acetone, benzene, phenol, toluene, chloroform, crezol, acetic acid, chlorate.
- If the instrument is wet, shut down the machine immediately, remove the power cord, and request for the technical service.
- Do not insert conductive or flammable objects into the air ducts formed inside or outside the instrument. There is a risk of fire or electric shock.
- Do not give a shock or vibrate the instrument.
- Avoid contact with pesticides or combustible gases.

4) Storage and Transfer

- Be careful when transporting the instrument since it is heavy. Use required and appropriate tools when transporting the instrument, two or more people should carry it together.
- Do not move the instrument with the door holding.
- Do not cause mechanical shock or vibration during the transportation and storage of the instrument. Internal damage may cause problems with operation.
- Disconnect the power plug when the instrument is not in use.

5) Cleaning

- Before cleaning, turn off the power switch and remove the plug from the outlet. There is a risk of electric shock.
- Also, wear chemical resistant gloves.
- Never use chlorine detergent. It may cause the chamber to be oxidized. Also, do not use volatile substances such as cleaning agents, abrasives, benzene, acids or solvents.
- Do not use organic solvents such as sulfuric acid or hydrochloric acid to wipe the surface of the instrument.
- Use a soft cloth or sponge with a neutral detergent to clean the cleaning tool.
- Do not pour water directly into the instrument while cleaning the instrument or its surroundings.
- Do not disassemble when cleaning the instrument.
- If you are cleaning the instrument in a way other than the above, please check the cleaning manner with JEIOTECH.

6) Repair

- The electric parts and circuits embedded in this instrument are developed by JEIOTECH, therefore no one, who is not JEIOTECH employee or delegated person, should never fix this instrument.



Avoid high frequency.



Avoid water.



Beware of electric shock.



Beware of heavy weight.



Beware of fire.



Wear gloves.

In addition to the above-mentioned safety warnings, safety warnings are mentioned throughout this manual. These safety warnings are described with "warning marks" and "safety warnings". If users do not follow these important instructions, they may cause severe defects or fatal damage to the instrument, may result in personal injury, and death.

2.0 Functional Description

2.1 Introduction

This instrument is a multi-purpose Forced Convection Oven that can be used in a variety of the fields such as biotechnology, pharmaceutical, medical, chemical, and biology. It is a fast-drying instrument that supports an excellent experimental environment of thermal curing and denaturation of samples, preheating of building materials and electronic components, heating removal of food, and experimenting heat resistance.

2.2 Feature

2.2.1 Excellent Performance

(1) Controlling wide range of temperature

It controls up to 250°C. An excellent insulation of the instrument minimizes heat loss inside the chamber.

(2) An excellent temperature uniformity and precision

The internal fan transfers the heat to the samples quickly, evenly, and precisely.

(3) A reliability and reproducibility of temperature

An excellent reliability and reproducibility of temperature distribution has been verified by strict overseas standards, DIN 12880 and IEC 60068-3-5.

(4) An excellent insulation and low heat loss

Mineral wool resin insulation of an external chamber and doors, and high-temperature silicone door packing supports an excellent insulation and low heat loss.

(5) Convenient control

Automatically sets the PID temperature control coefficient suitable for the user's operating environment. [4.5.3 Refers to Auto tuning].

(6) Precise temperature control

A 3-point temperature correction function enables calibration of three temperature points to ensure accuracy in a wide temperature range. [4.5.2 Refers to Calibration]

(7) Automatic temperature suggestion system

Even though the user does not save any specific temperature value, the system suggests three frequently-used temperatures automatically.

(8) Automatic event-recording system

It automatically records up to 36 alarms that are occurred while using the device.

(9) Ramping function of temperature

If the temperature-changing rate is set in the basic mode, the internal temperature of the chamber can be heated slower than the maximum heating rate.

2.2.2 Safety Enhancement

(1) Emergency management with a CLS-Control System

The CLS (Custom Logic Safety)-Control System is industry's first implementation that enhanced convenience, safety, and stability specifically in laboratories with various flammable drugs. The CLS system (Patent Registration No. 10-0397583, 10-0328729) immediately cuts off both phases of power completely supplied to various parts of the device, with notifying the user of an unstable operation with a visual and audible manner, and keeps the device powered off until it is manually restarted by an operator. It is developed by its researchers for the safe use of heated devices operated in environments that require perfect thermal safety, such as.

(2) Overcurrent limiter

Safety circuit protect the device from overcurrent and over-heating of the heater.

(3) Over temperature limiter

An embedded mechanical temperature limiter prevents damage from overheating. [4.7. Refer to Over temperature limiter]

(4) Viewing window (OF4-PW model)

OF4-PW model is a triple pane transparent window enhanced an excellent insulation while securing an easy observation.

(5) Check for during operation.

When an abnormality occurs during operation, the error content is displayed on the screen and the alarm sound is activated.

(6) Instantaneous Outage Recovery Features

If the instrument has a short period of power outage occurs within 30 seconds, the system returns to the previous operating status. [4.2.8 Instantaneous Outage Recovery Features]

2.2.3 Improved Convenience

(1) 5inch LCD display with a touch controller

5inch display secures an improved visibility and usability supported by a convenient touch screen.

(2) Start reservation, end reservation timer setting

You can schedule to start temperature control after the entered time. Once the temperature reaches to a target value, you can also set the timer to terminate the temperature control. [4.2.3 Refer to Timer Settings and Control]

(3) Program function

10 programs can be set, and 10 steps and 99 repetitions per program can be set to set various experimental conditions. You can skip a step in progress or keep the current step.

(4) Scheduler

It provides a scheduler function that enables reservation execution by selecting the desired day, time, and program.

(5) Auto-run function

The auto-run function saves the previous temperature settings for the system recovery from a power outage for more than 30 seconds. [4.4.4 Refer to Auto run & Door lock]

(6) Screen lock function

You can active the screen lock function by touching the lock button at the top during the operation. Press the lock button once more to unlock the controller screen.


(7) LC-Connected service (option)

A remote controlling and monitoring system, LC-GreenBox (option), enables the users to control and monitor via smart devices. You can also enroll in a separate service to store and provide 30-day monitoring data.

(8) Double stacking (05,15 only option)

The space utilization is excellent because it can be loaded in double stacking using a bracket. It can also be mixed with OF4/ON4-S, V-type of the same size.

2.3 Structure

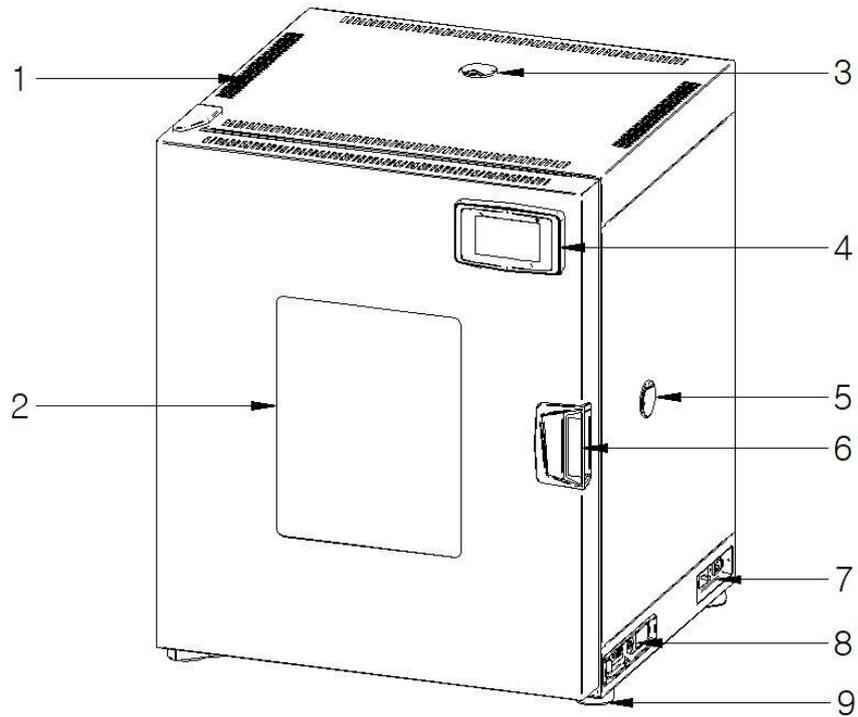


- (1) Main body
The main body is made of iron plate and painted with coatings.
- (2) Viewing window (Option)
The triple-pane window is transparent to improve excellent insulation and easy internal observation.
- (3) Exhaust vent
It is an outlet for letting the air exhaust from the chamber. If you would like to adjust the amount of air to be exhausted, please turn the vent hole cover.

WARNING



- Since the instrument is in excessive heat, please wear gloves when controlling the vent hole cover. If you use wet gloves, it can cause burns on the hands, since it speeds up the temperature conduction of the high-temperature part.
 - When a short circuit occurs due to aging of the device, never wear wet gloves or bare hands, since the operator can be electrocuted.
-

(4) Controller & USB port

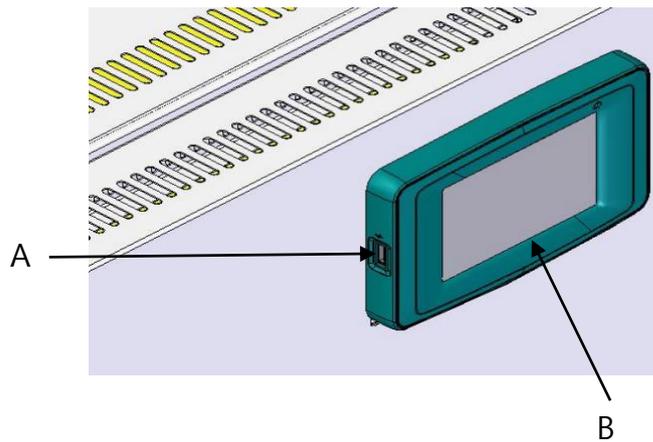

[OF4, Controller]

A) USB port

It is a USB port used to store data and is located on the left side of the controller. [4.2.8 Refer to USB storage function]

B) Controller

It is operated with a 5-inch touch screen and has built-in electrical components.

(5) Ventilating hole

To control the amount of air to be exhausted, you can use the ventilating hole.




WARNING

- The instrument is in excessive heat, therefore please wear gloves when controlling the exhaust. Wet gloves can cause burns on the users' hands, since it speeds up the temperature conduction.
- Also, wet gloves or bare hands are not allowed, since the operator can be electrocuted when a short circuit occurs due to aging of the device.

(6) Door handle

The door handle can open or close the door.

(7) Side panel-1

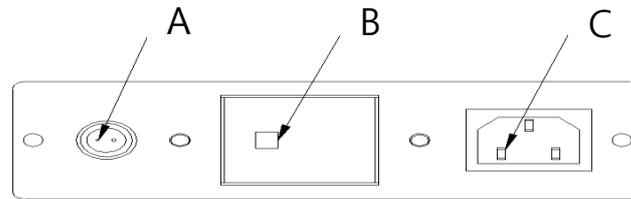

A) BMS connection port (Option)

The embedded BMS connection port is a circular connector-2pin type. By using the BMS (Building Management System), it is possible to quickly respond to an abnormality by monitoring the temperature of the product on the building management system. The connector specification is SCN 16-02R, and the output specification is 4~20mA, and the temperature of OF4-P is transmitted to the BMS.

If BMS connection port is not selected as an option, a rubber plug  is attached.

Ex) The temperature range of OF4 is 0 to 250 degrees, and when the temperature of OF4 is 125 degrees, 12mA is output.


B) Circuit breaker

A circuit breaker is embedded to protect the device from short circuits or overcurrent.

C) Power cord socket.

The socket connects the power line to the instrument.

(8) Side panel-2

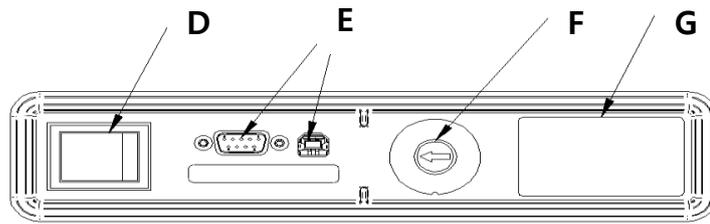


D) Main switch
It turns on and off the main power.

E) Communication port (Option)
The USB port and the RS232 port connects the device to a computer to monitor or operate the instrument. When connecting both ports at the same time, the USB will be recognized firstly.

F) Over Temperature Limiter
If the heat rises excessive temperature, the temperature control stops, and a warning sign will be displayed on the screen along with a notification sound. Once you check the warning sign, please solve the problem, and reset the Over Temperature Limiter up to 15% higher than the original target temperature. You can restart the instrument by pressing the Start button.

G) Product Label
The label describes the instrument name and its type.

(9) Foot
It supports its body and prevents slipping.

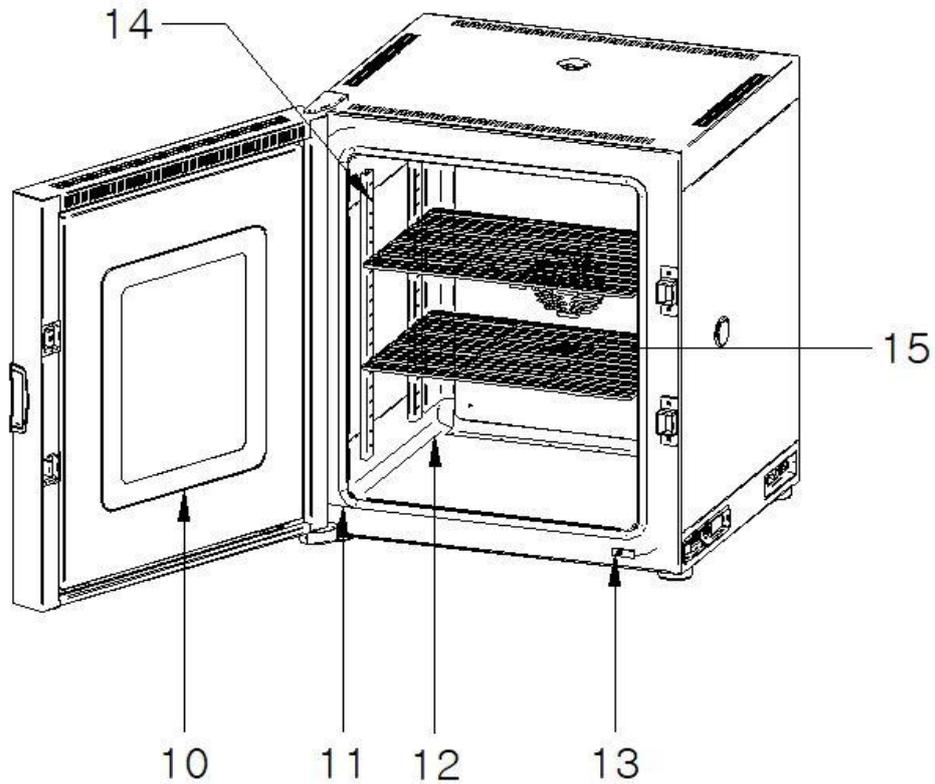

(10) Door

Space between door surface and the internal insulation part protects the door from being heated.

(11) Door packing

The door is packed with high-temperature silicone rubber to maintain airtightness.

(12) Chamber

The chamber is made of stainless steel. Inside the chamber, a fan, heater, temperature sensor, and temperature regulator are installed.

(13) Door limit switch

Door limit switch detects the opening and closing of the door. Once the door is opened, the controller stops the fan and the heater. If the door is opened for more than 2 minutes, the displays will show you an error message with an alarm sound. Moreover, the instrument operation will be stopped with the power disconnection with the Magnet Contact (MC).

(14) Shelf level adjuster

The shelf level adjuster easily enables for the shelf to adjust its height. OF4-03P(W) can be adjusted to 9 stages, OF4-05P(W) to 11 stages, OF4-10P(W) to 17 stages, and OF4-15P(W) to 19 stages. But for safety, it is recommended to install one shelf for two height adjustment holes for safety. Please refer to 9.1 Technical Specification for the maximum number of shelves.




(15) Shelf

Using shelf, you can place samples on it. Wire/Performed shells can be selected according to the type, characteristics, and size of the sample.

3.0 Installation

3.1 Components of the Instrument

Please check all the components described in this manual after unpacking. Also, please check the ID label attached to the instrument and make sure it matches the model you ordered. If there is any component below that does not match with your order, please contact the branch or device seller of JEIOTECH. Please refer to the 9.4 contact point information of our company.

Item	Figure	Quantity	Description
Unit		1	-
Shelf		2	-
Shelf Support (Please refer to 3.2.4)		8	-
Main cord		1	-
Operation manual		1	-

3.2 Preparations before installation

3.2.1 Installation Condition

Please follow the install guidelines between for your safety.

WARNING



- Do not install any gas pipe or water pipe around the instrument.
- Do not install in places with a risk of high humidity, short circuits, leaks, or flooding.
- If moisture or organic solvents flow into the control panel, short circuit may be occurred.



- Do not install the instrument in a place with a possibility of flammable gas leakage.
- Do not use or store flammable dust, combustible gas around this instrument.
- Operation of the device is prohibited in a place with a possibility of explosion due to organic evaporation gas.
- Do not use the device in places with industrial harmful gases, fumes, or metal dust.



- Do not expose the instrument to direct heat sources or direct sunlight.



- Maintain the temperature around the device at 5°C to 40°C.
(The optimal temperature is 25°C.)



- Please keep the relative humidity below 80%.



- Install the device in a place below 2,000m above sea level.
-



⚠ CAUTION



- Do not install near instrument that generates strong high-frequency noise (high-frequency welding machine, high-frequency sewing machine, large-capacity SCR control).
 - Please beware of using artificial heart pulses or magnetic data devices which may be affected by magnetic bars.
 - Do not install any electrical instrument near the power terminals.
 - Do not avoid unventilated corner. If ventilation is not sufficiently performed, heat dissipation will be in a risk of damage due to overheating.
 - The instrument should be installed near the power outlet.
-

3.2.2 Installation Guidelines

Please follow the guidelines listed below.



⚠ WARNING

- Please install the instrument on a flat and solid floor for any case of an accident.
 - Since the door is opened to the left with maximum 115°, please consider sufficient installation space.
-




⚠ CAUTION

- Please keep the appropriate space (typically at least 30 cm) between other devices or walls.
-

- (1) Please install the instrument inside the laboratory with a little human access.
 - (2) Install it horizontally on a solid and flat floor.
 - (3) Install it in a place without any direct sunlight and heat sources.
 - (4) Please install it in a place without water or steam effect.
 - (5) It is recommended to install it in a place where there is an exhaust system such as a fume hood or an arm hood.
 - (6) Please keep a certain space from the wall or other adjacent experimental equipment.
- In particular, the door of the device opens in the left direction, please make sure to have enough space on the left so that the door can be fully opened.

3.2.3 Minimum required space for Installation location

In order to install the instrument, you need to consider the size and rotational radius of the instrument. When installing it, you should keep a minimum space of the product to operate and maintain properly as shown in the figure below. It is also recommended to install it in an environment equipped with ventilation facilities such as a fume hood or arm hood.

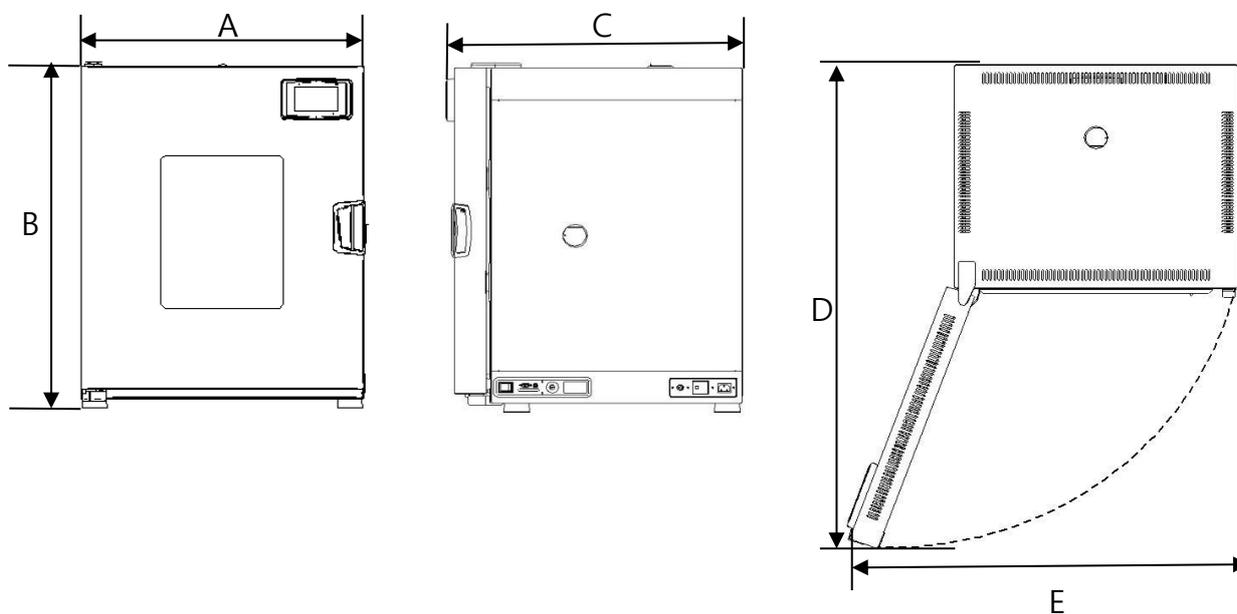

Model Description		OF4-03P(W)	OF4-05P(W)	OF4-10P(W)	OF4-15P(W)
		A	Exterior width	478	558
B	Exterior height	604	684	859	914
C	Exterior depth	527	648	677	704
D	Maximum depth with door open	868	1060	1185	1271
E	Maximum width with door open	695	809	958	1050

(unit: mm)




CAUTION


- Please avoid samples or shelves contacted to sensors.

3.2.4 How to install shelf and its support

You can adjust the height of the shelf by attaching the shelf support to the shelf adjustor on the side of the chamber as shown below.

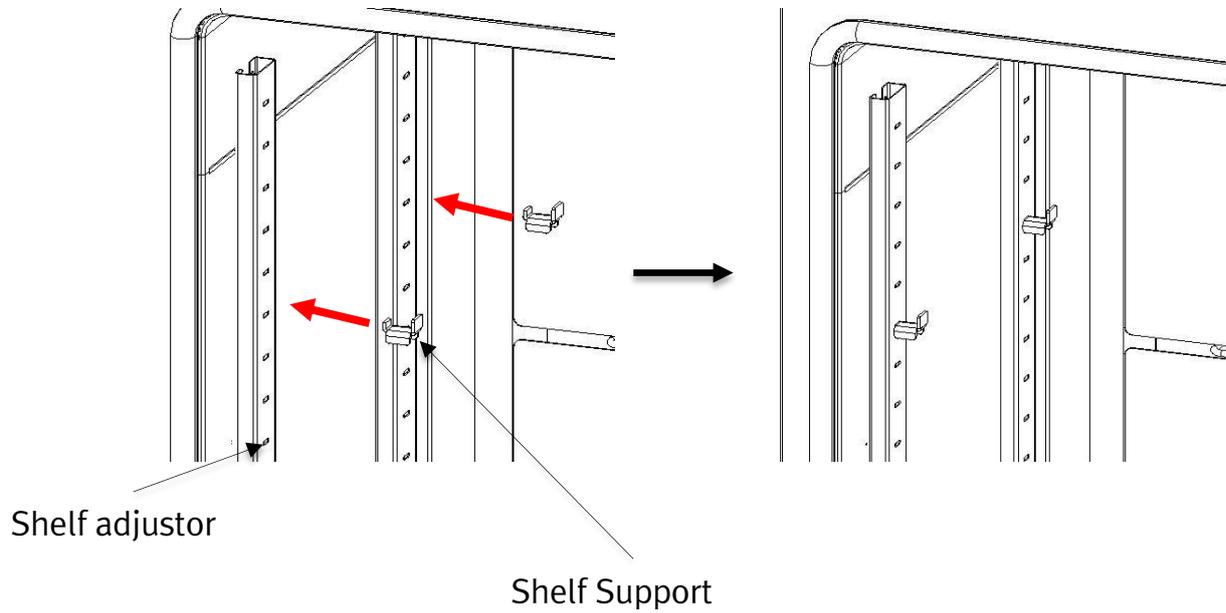


Place the shelf on the shelf support attached to the shelf adjustor. Depending on the model, up to 4 to 9 shelves can be installed.

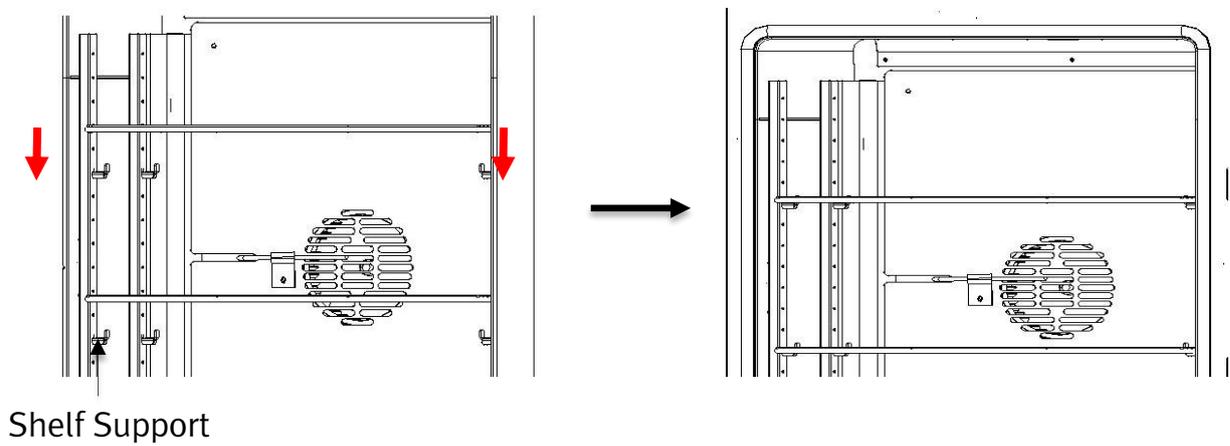

3.2.5 Available Space

Please make sure the available space around the instrument.

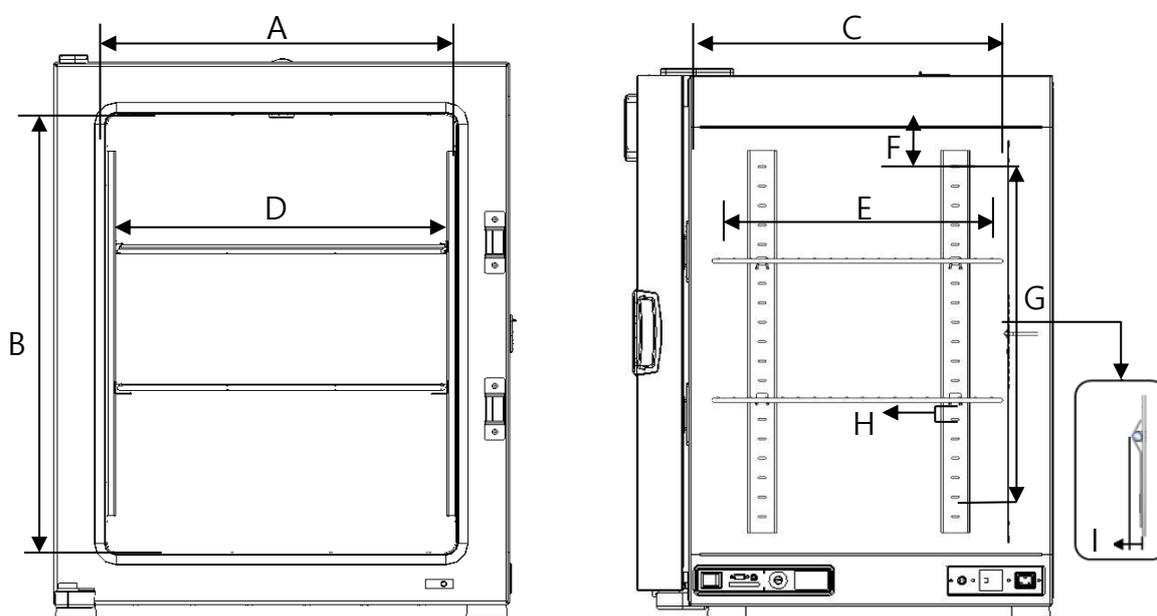

Description		Model			
		OF4-03P(W)	OF4-05P(W)	OF4-10P(W)	OF4-15P(W)
A	Interior width	300	380	485	550
B	Interior height	400	480	655	710
C	Interior depth	210	330	350	376
D	Shelf width	266	346	451	516
E	Shelf depth	195	315	335	361
F	The height between the top hole of the shelf installation and the inner top	80	90	87.5	85
G	Height between the top hole and the bottom hole of the shelf installation	240	300	480	540
H	Spacing of Shelf installation Holes	30	30	30	30
I	Sensor installation depth	3.8	3.8	3.8	3.8

(unit : mm)



CAUTION

- Please avoid the contact between sensor and self/ samples.

3.3 The labels attached to the instrument

1) ID label

An ID label of the basic information is attached on the panel of the right side of the instrument. Before using it, please check the voltage, phase, and capacity of the power indicated on the ID label.

2) Safety label

Safety labels are attached to the instrument to provide important information about potential risks or how to avoid them. For safe operation, all users must check the safety label before using it and read the 1.4 Instructions for Safe Use (required reading) carefully to understand the relevant safety guidelines. If the safety label is damaged, please ask the JEIOTECH branch or seller for a new label.

3) Custom Logical Safety (CLS)-Control System Label


It is a label that certifies that the CLS-Control system, the highest safety level control device, is applied. [2.2.2 Refer to Safety Enhancement]

Safety Label

경고 폭발 및 화재 위험 기기 내부에 폭발성 물질이나 가연성 물질이 넣지 마세요.		WARNING Explosion and Fire Hazard No explosive dust or flammable materials in the chamber.
주의 부식성 물질을 기기 내부에 넣지 마세요.		CAUTION Do NOT place corrosive materials in the chamber.
주의 표면 고온 화상을 입을 수 있습니다. 취급 시 주의하세요.		CAUTION Hot Surface Do NOT touch. Contact may cause burn.



CLS-Control system Label

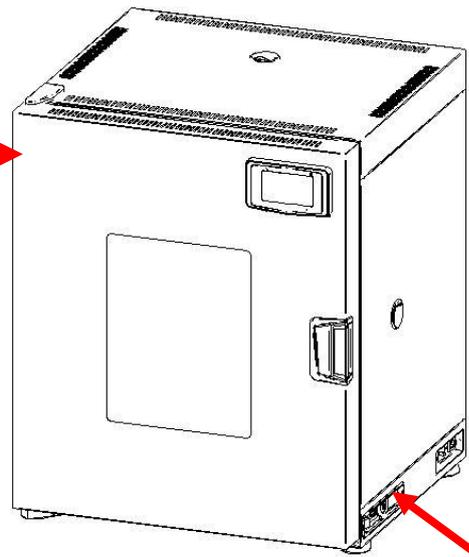

Code No.	XXXXXXXX
Description	Forced Convection Oven
Model	OF4-XX(W)
Voltage	XXX
Serial No.	XXXXXXX
JEIOTECH www.jeiotech.com	
CE Made in Korea	

3.4 Power Connection

1) Before connection to a power, please follow the guidelines listed below.

WARNING



- Before installing the product, please check the voltage, phase, and capacity of the power and connect it correctly.
- Make sure to use a power source with a grade 2 or higher ground. Also, never ground it to a gas pipe or water pipe.
- Do not connect to one outlet and use it with other devices at the same time.
- Never use branch sockets or double tabs. In the event of an overcurrent, there is a risk of damage to the cable, damage to the device, and fire.
- Operation of the device is prohibited when there is damage to the power line.
- Inappropriate power connection can cause damage to the device and serious injury or death to the human body.
- Do not handle or touch electrical cord or electrical components with wet hands.


CAUTION



- When installing and operating, please make sure to use the outlet provided with the ground terminal for the power cord.
- Accurately fasten the power plug so that it does not shake.
- Avoid placing heavy things over the power cord or let the cord pressed under the device.
- After use, please be sure to turn off the main power switch and unplug the power cord.

2) Please follow the step-by-step guidelines to supply power to the instrument.

- (1) Make sure the power switch, circuit breaker is off before supplying power.
- (2) Connect one side of the power plug to the power input terminal on the side of the body.
- (3) Connect the other side of the power plug to a power outlet.
- (4) Turn on the power switch and circuit breaker to supply power to the device.

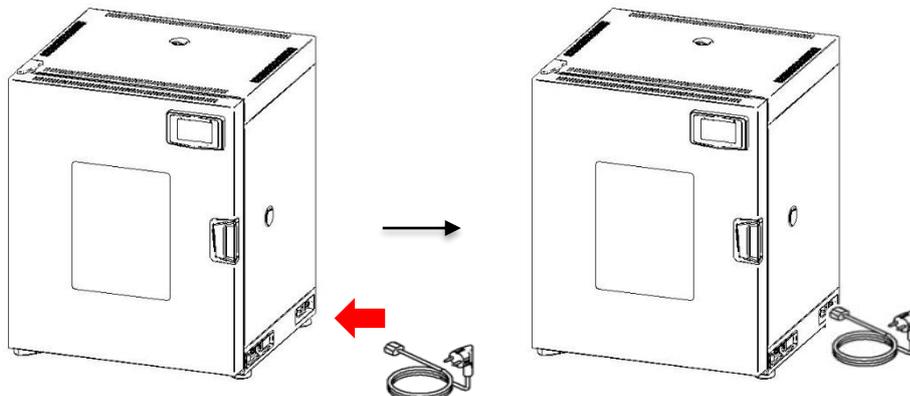

3.5 Checklists before the Use

When operating the instrument, please keep the following warnings.

(1) Warnings for use of chemical materials



WARNING



- Do not put any substances that can cause toxic gas inside the instrument.
 - Do not put flammable dust inside the instrument. If combustible dust enters the heater, it may cause a fire or explosion. This device is not an explosion-proof structure.
 - Do not place explosive, flammable, flammable, or oxidative chemicals such as alcohol, benzene, gasoline on top of the device, store them, or put them in the instrument and operate them. There is a risk of fire. This device is not an explosion-proof structure.
-

(2) Warnings for Use of the Instrument



WARNING



- Do not operate devices that have been damaged or have short circuits.
 - Do not use the device if strange sounds, smells, or smoke occur on the instrument.
 - Make sure to wear safety equipment (work clothes, gloves, safety goggles).
-

(3) Warnings for instrument damage

WARNING



- Avoid moisture, organic solvents, dust, corrosive gases entering the instrument.



- Do not place a liquid-storing container on the top of the instrument. Spills of liquid may cause damage to the instrument.
-

(4) Cautions for the Use of the Instrument

CAUTION



- Please wear gloves when handling samples to avoid burns, as there may be residual heat even after the power is off.



- Before using the instrument, please make sure the inside of the chamber is clean all times.
- If this instrument has moisture, please stop operation immediately, disconnect the power cord, and request for a technical service.



- Do not put conductive or combustible objects inside the vent pipe. There may be a risk of fire or electric shock.


- Be careful not to damage accessories or systems inside the instrument.
- Do not give a strong shock or vibration to the instrument.




- Avoid contact with pesticides or flammable gases.
-

3.6 Stacking Set (Option)



When stacking two products of the same size, the Stacking Set allows for efficient use of space. It is only available for products sized 05 and 15. The components and installation method for the Stacking Set are as follows.

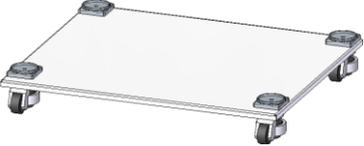Item		Figure	Quantity
Roller Base			1
Bracket 1			3
Bracket 2			1
Housing panel			2
Rear Bracket 1			2
Rear Bracket 2			2
Truss Head Tapping bolt	M4x8		8
	M4x20		3


- (1) Position the Roller Base in the direction shown in the picture. Fix the Caster and align it horizontally, and load the product to be located at the bottom on the Roller Base in alignment with Bracket 1.

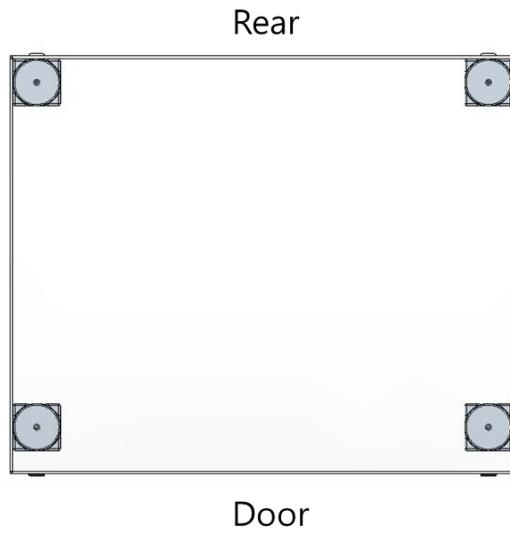


- (2) Insert the Housing panel from the front of the lower product, and separate the two bottom bolts of the product.

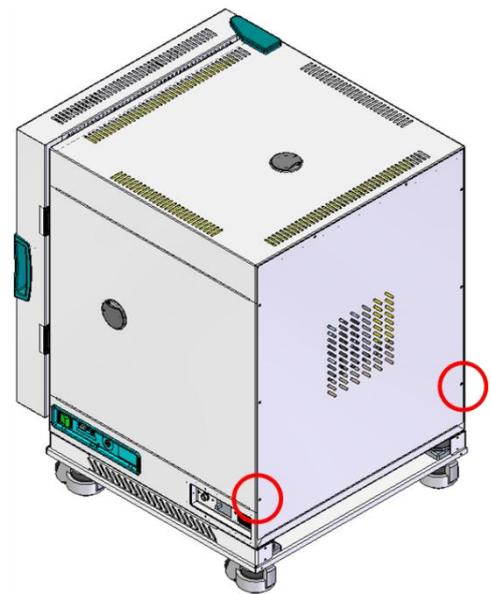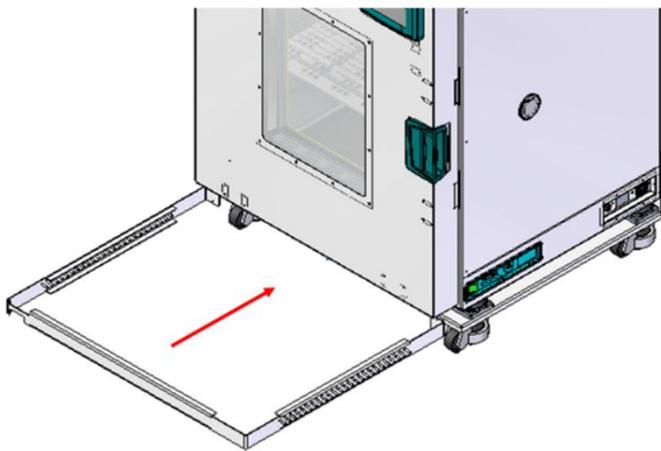


- (3) Attach the Rear Bracket 1 in the direction shown in the picture using the Truss Head Tapping M4x6 bolt.

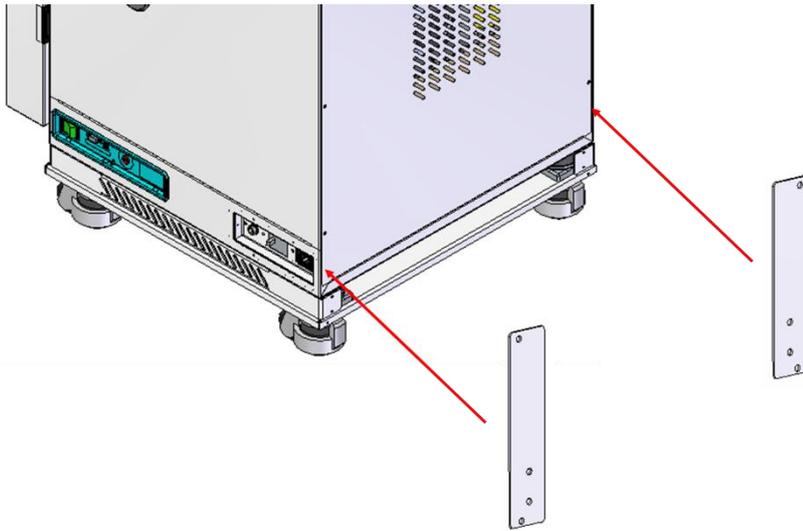


- (4) Attach the Bracket 1 to the lower product using the Truss Head Tapping M4x20 bolt with an electric drill torque 1, and insert the hinge into Bracket 2 as shown in the picture.

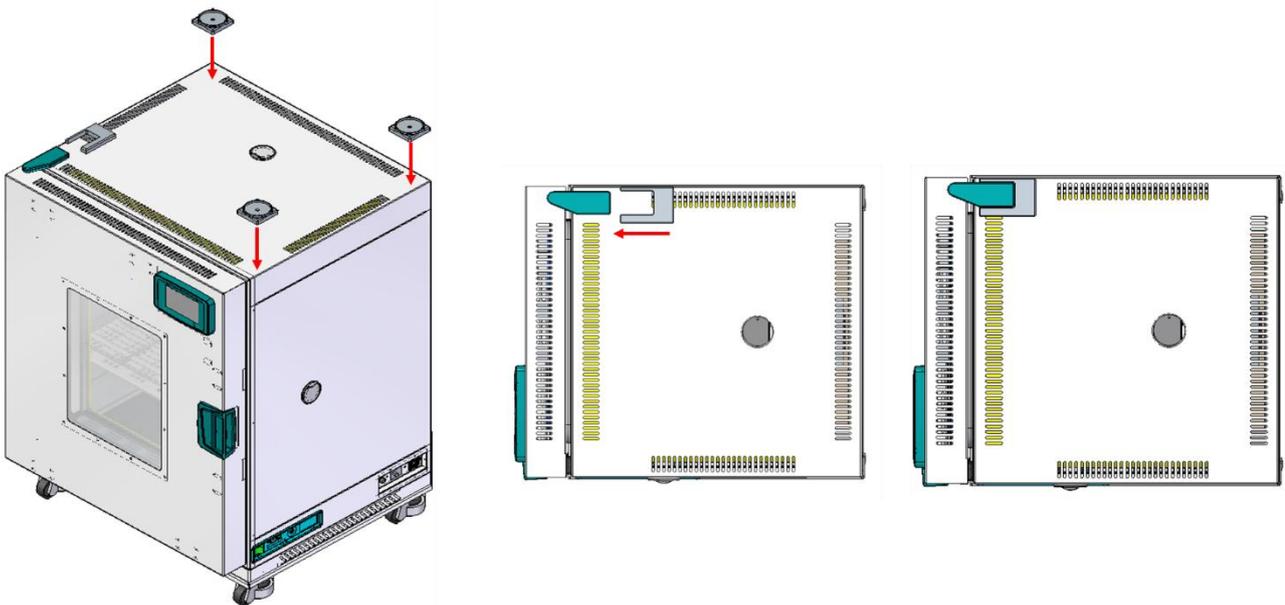

- (5) Load the upper product in alignment with Bracket 1. Lift the front of the upper product and insert the Housing panel from the front.

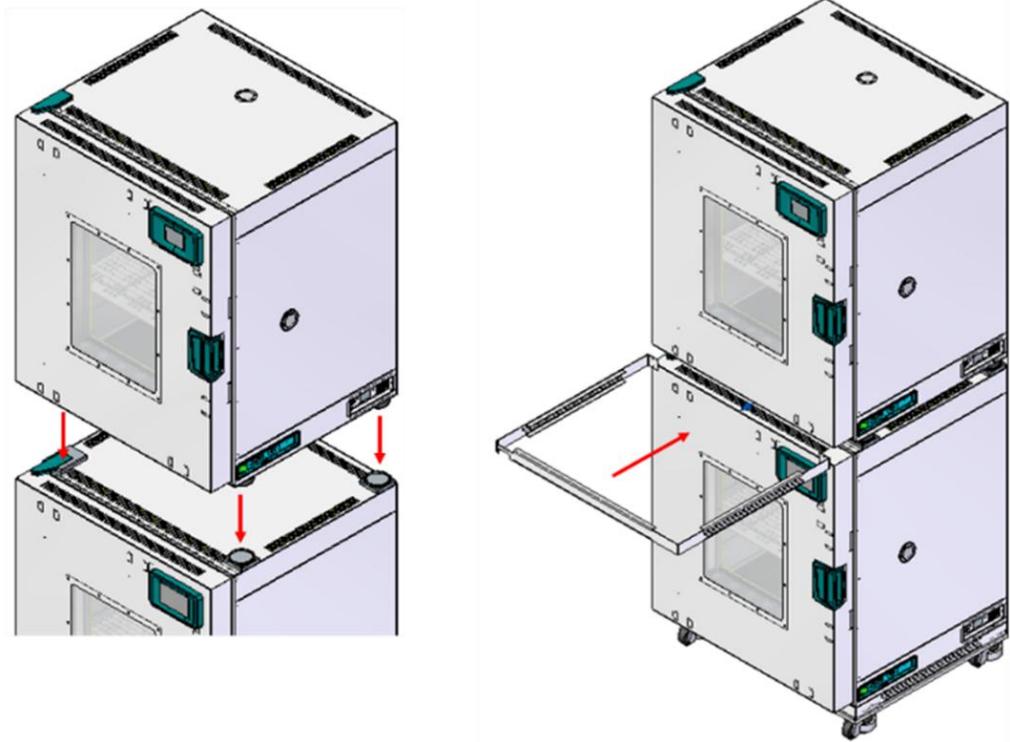

- (6) Remove the two bottom bolts of the upper product, and attach the Rear Bracket 2 in the direction shown in the picture using the Truss Head Tapping M4x6 bolt.

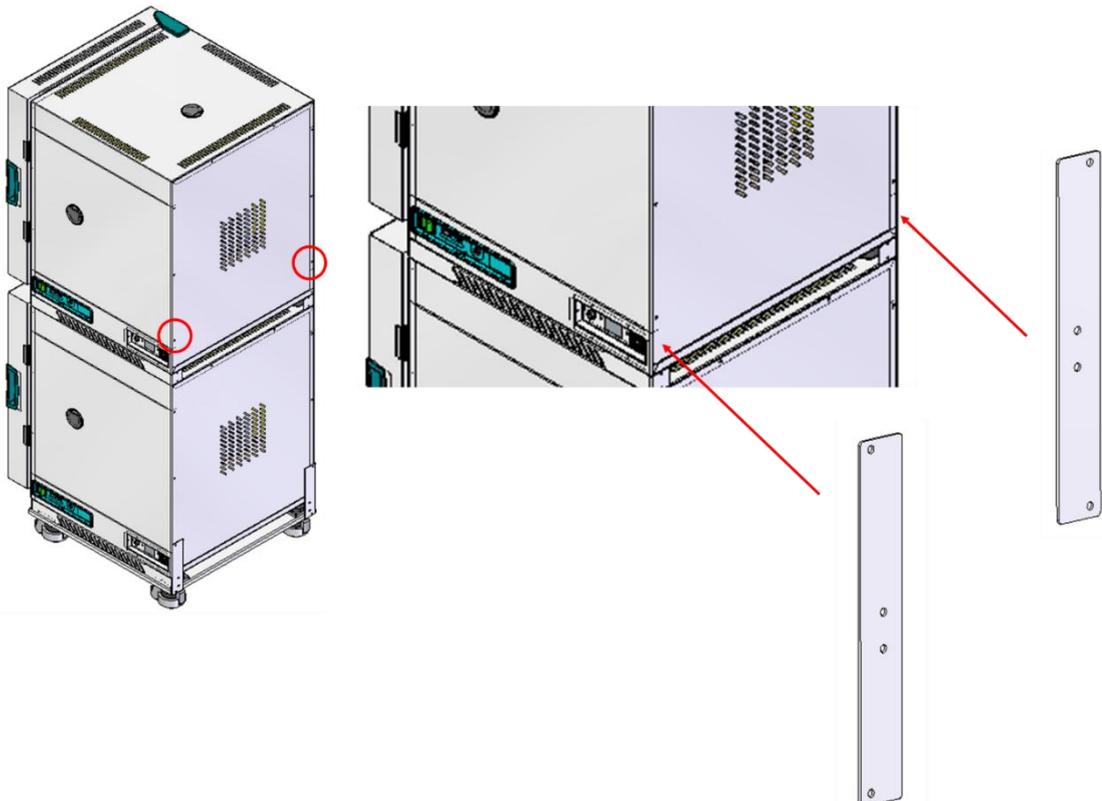

⚠ CAUTION


• Chamber of the same size using a Stacking Set can greatly increase laboratory space efficiency. However, the minimum control temperature of the upper chamber may be limited due to the heat generated by the lower chamber as shown below.

1. When placing the oven on the bottom and the incubator on the top: The temperature range of the upper incubator can increase by up to $\text{amb}+25^{\circ}\text{C}$, depending on the set temperature of the lower oven.
2. When placing ovens at both the top and bottom: The temperature range of the upper oven can increase by up to $\text{amb}+25^{\circ}\text{C}$, depending on the set temperature of the lower oven.

• Therefore, to ensure the minimum control temperature of the upper product, it is recommended to use the lower product at a low temperature and the upper product at a high temperature.

4.0 Operation

4.1 Controller Home Screen names and functions

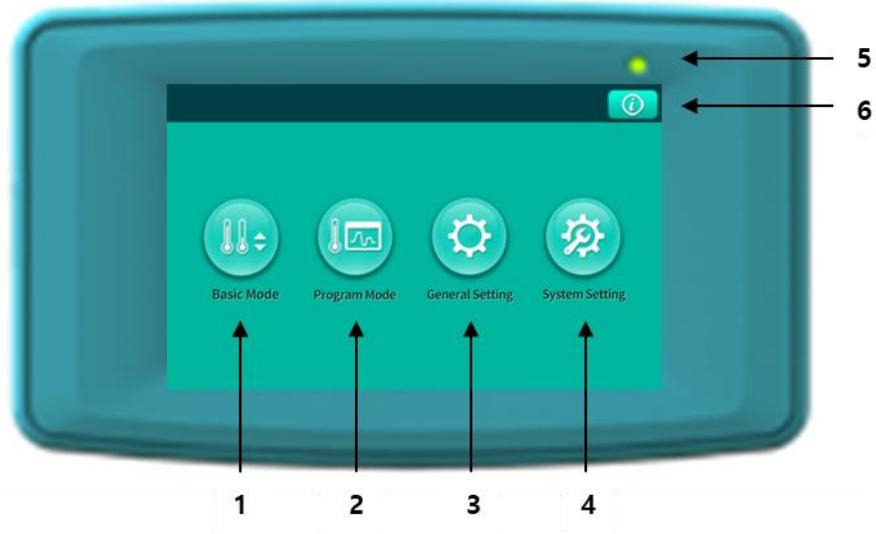


	Menu	Functions	Chapters
1	Basic Mode	Temperature can be controlled with temperature settings, timer [start reservation, end reservation], temperature control and stop, and temperature change rate functions.	4.2
2	Program Mode	Temperature can be controlled with by setting the target temperature, timer, number of program cycle, and the program shutdown function.	4.3
3	General Settings	You can check and change the settings of the device, such as sound settings, date/time modification, and language selection.	4.4
4	System Settings	You can set and change the alarm settings, password settings, factory initialization, etc.	4.5
5	LED Indicators	Even when the screen is automatically turned off, you can check whether the current device is operating or not via the upper green LED display.	-
6	Information	You can check the version, model name, and information of the firmware.	-

4.2 Basic Mode

Basic mode is used when the user controls the temperature inside the chamber by one temperature point. You can change the target temperature and timer value before and during the instrument operation.

Press the Basic Mode button  on the home screen to go to Basic Mode.

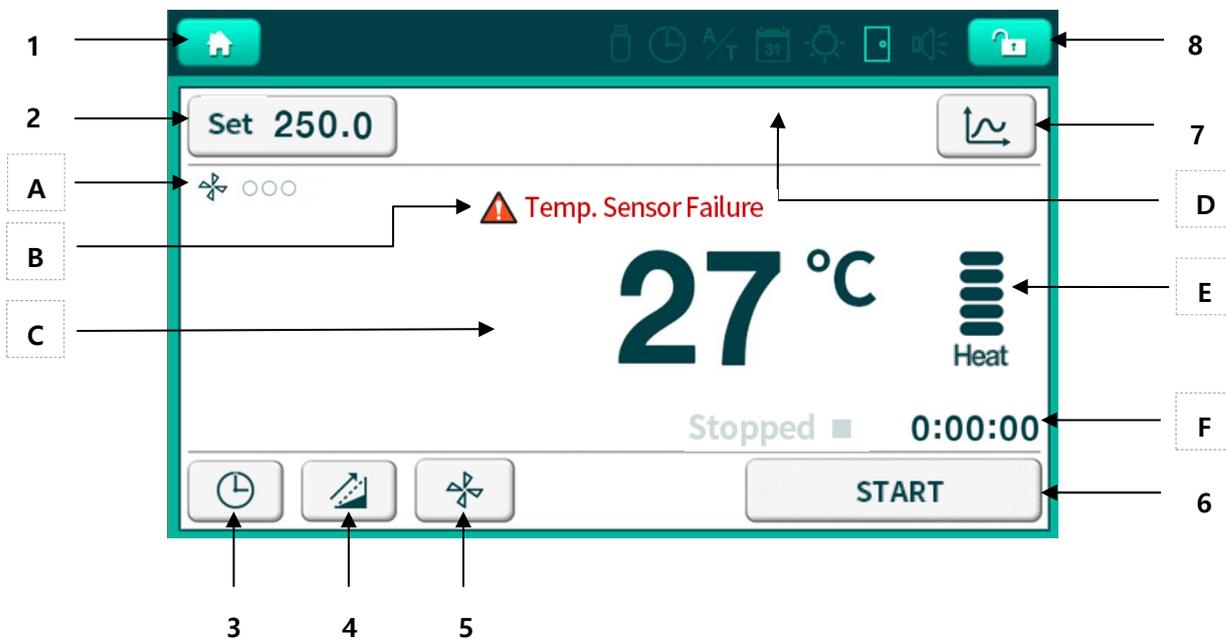

[Window for operating status in Basic Mode]

(1) Status Display

A	Fan	Displays the set speed among the three stages of the fan's speed.
B	Warnings	When a warning occurs, an alarm sign appears, and a pop-up notification window appears.
C	Current Temperature	Indicates the current temperature inside the chamber.
D	Operating Status	<ul style="list-style-type: none">  Auto Tuning  Setting Timer  Door Open/ Close  Sound On/ Off


		 USB connection  USB not recognized  Data transfer via USB
E	Heating amount	Displays current heating amount
F	Operating status and running time	Depending on the operating status, it displays the operating time or remaining time of timer with the phrases in operation, start reservation, and reservation, and running, stopped.

(2) Button

1		You can move to home screen. (When the power is turned on, it automatically enters the basic mode. You can use this button to make general and system settings.)
2		You can set the target temperature value.
3		Timer Setting: You can set the start/ stop timer.
4		Ramping rate: You can control the rising rate of the temperature between 0 ~ 50°C per min. (Unit: °C/min)
5		You can select the fan speed according to the characteristics of the sample, among the three stages.
6		It is a button to start temperature control and the text will be changed to "STOP" once the instrument starts.
7		You can move to Graph screen.
8		Screen lock On/Off

4.2.1 Start and Stop in the Basic Mode

If the device temperature control is stopped, you can start the temperature control by pressing the start button on the touch screen. When finished, press the stop button on the touch screen to stop the temperature control of the device.

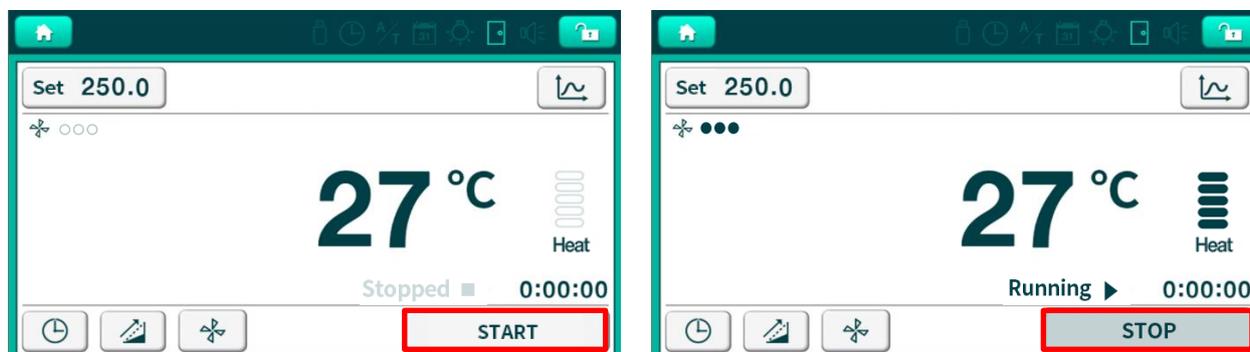


NOTICE

- If you try to control the instrument when the doors is opened, it will not operate with a door-open sound. Please close the door and restart it.
- If the door is opened while the device is operating, the fan and heater will stop operating, and a door-open warning message will be shown without a notification sound. If the door is closed within the 'Door Open Delay Alarm' time entered in System Settings > Alarms [4.5.4 Refer to Alarm], the previous operation continues. If the door is not closed within the entered time, a warning sound is issued a pop-up will appear. When the warning pop-up is displayed, the instrument will not work even when the door is closed. To restart the instrument again, please close the door, check the warning sign, and restart the instrument.

4.2.2 Temperature Settings

(1) On the home screen, press the Basic Mode button and press the button  on the upper left.

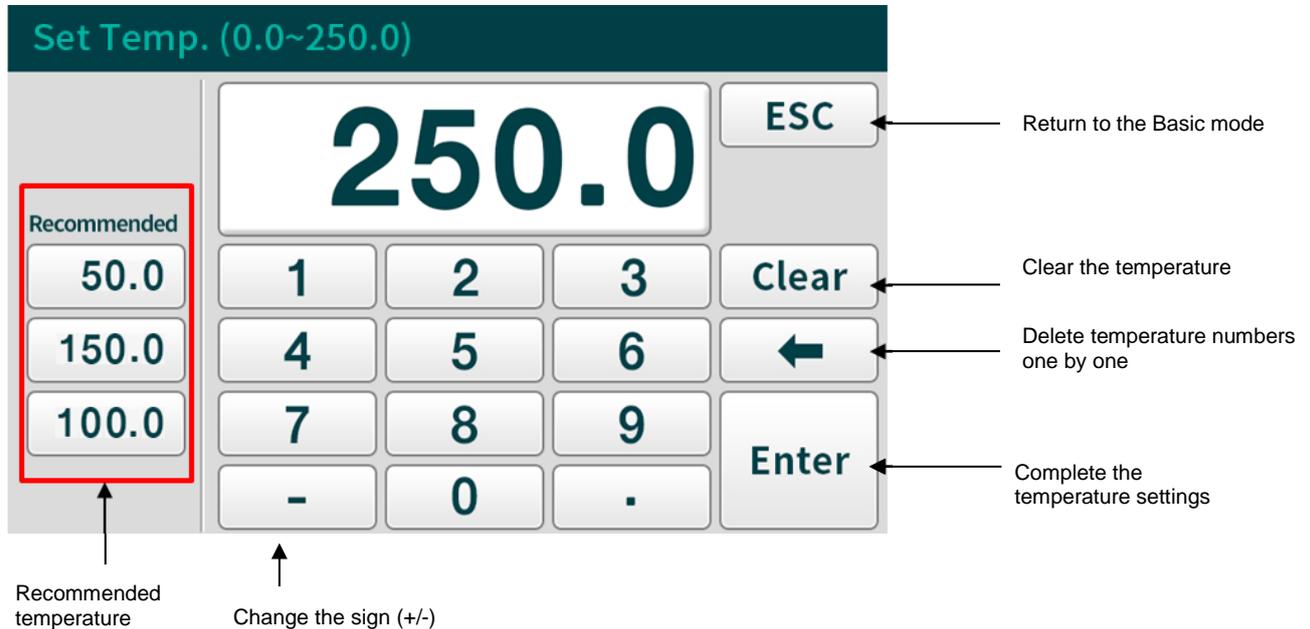

(2) When you enter the temperature settings, press the keypad to change the temperature value of the desired temperature. Press Enter to return to the basic mode. (If you press the ESC button without pressing Enter, the temperature settings will be canceled.)

※ Recommended temperature function

Three frequently-used temperature will be recommended and displayed. If you select one of the recommended temperatures and press the button, it will be set as the target temperature.

NOTICE


- The set temperature can be input from 0 to 250°C, and the temperature control range of the device is Amb. +10 ~ 250°C
- To set and start the temperature control, please press the start button.
- When the set temperature is changed through (1) to (2), the temperature control will start immediately to reach the target temperature.
- The frequently used temperatures are automatically saved and suggested.

4.2.3 Timer Settings and Control

This instrument has a wait on timer function to control the temperature control of the device after a set time. And after reaching the set temperature, there is a wait off timer function to control the temperature maintenance for a set time.




- (1) Move to Timer Settings by pressing the button,  in the Basic Mode.

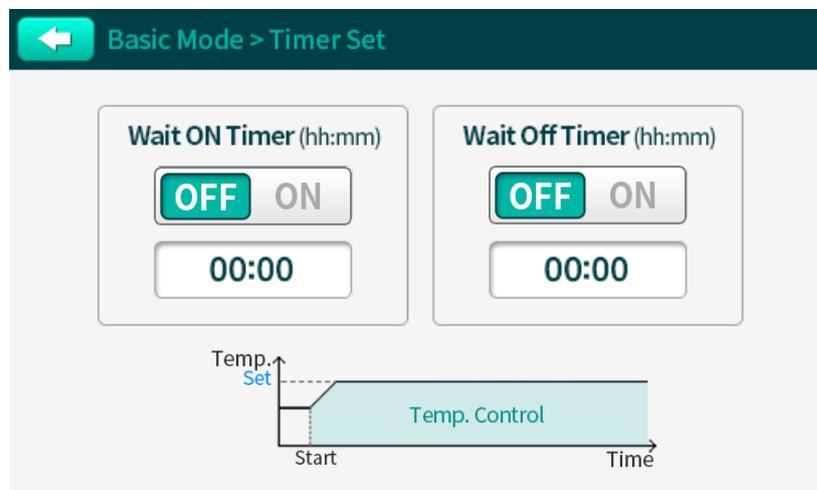


[The main menu of the timer settings]

- (2) Press the ON button of the “Wait ON Timer” and “Wait OFF Timer” you want to set.
- (3) Enter the “Timer Set” with the unit of “hh:mm”.

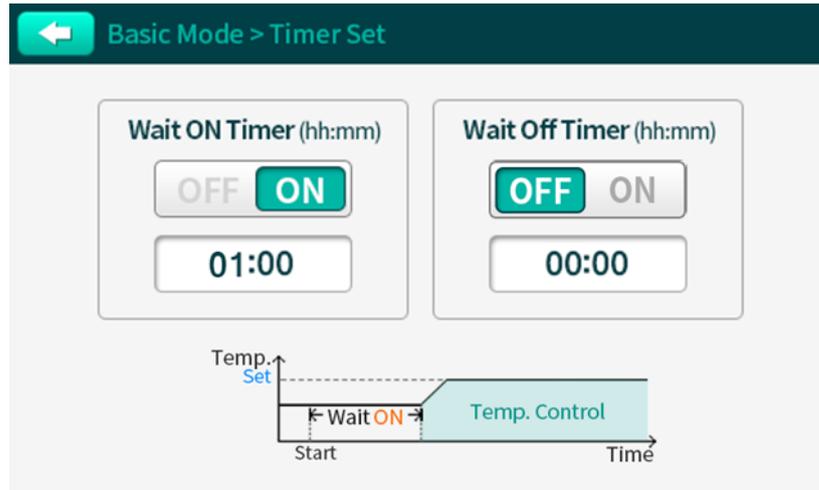





[In case setting the start timer as 1 hours]

- (4) You can return to the “Basic Mode” screen by pressing  button with the Wait ON/OFF timer applied. When the timer setting is completed, the icon,  will be shown on the screen.

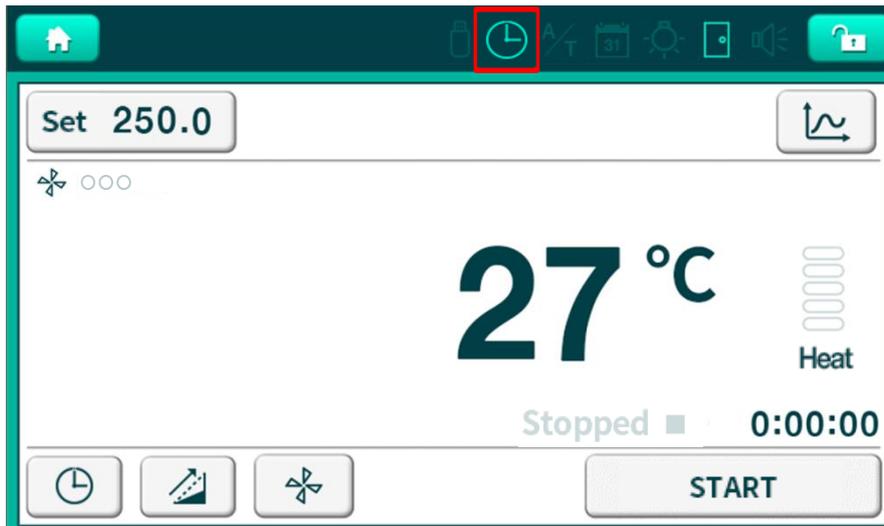


NOTICE

How to reserve the Wait ON/OFF timer

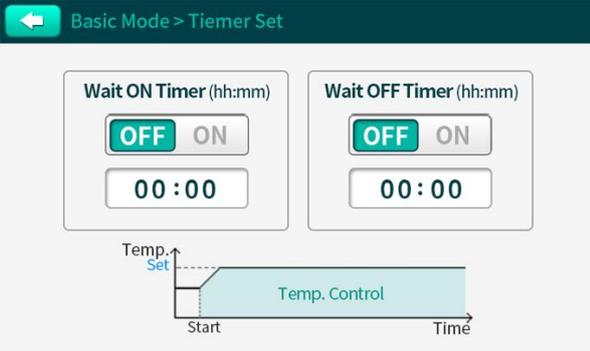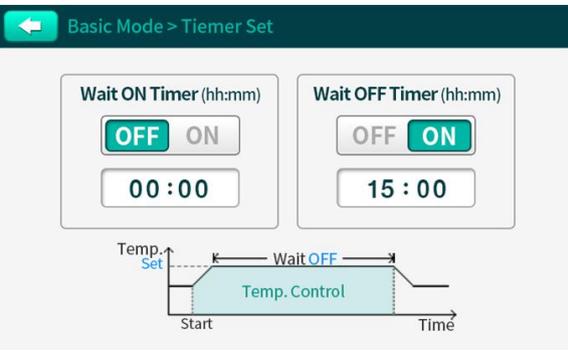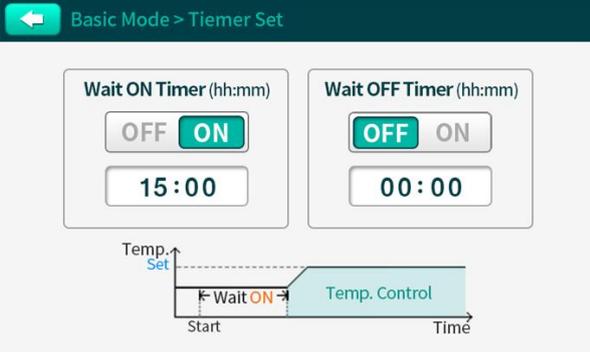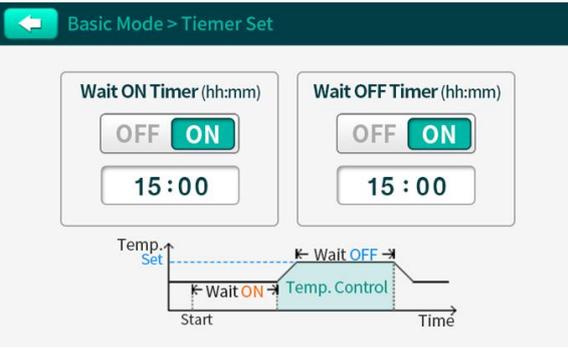
<p>In case of Wait ON Timer is OFF / Wait OFF Timer is OFF</p>  <p>- The initial setting is shown as above. - Timer set does not apply to this instrument.</p>	<p>In case of Wait ON Timer is OFF / Wait OFF Timer is ON</p>  <p>- If you only set the Wait OFF timer, the temperature will maintain only for the entered time once it reaches the target temperature. - The temperature control will be terminated if all the reserved end time is passed.</p>
<p>In case of Wait ON Timer is ON / Wait OFF Timer is OFF</p>  <p>- If you only set the Wait ON Timer as ON, the instrument waits for the input value before raising the temperature as the set value. - In this case, the heater will be continuously working to maintain the set value until the user stops the instrument.</p>	<p>In case of Wait ON Timer is ON / Wait OFF Timer is ON</p>  <p>- If you turn on both Wait ON Timer and Wait OFF Timer, you can set the delay time before starting the heater and also set the maintaining time to last the set temperature. - In this case, the heater operation starts after all the time set in the Wait ON has elapsed. After reaching the target temperature set by the user, the target temperature is maintained for the time set by the Wait OFF. Temperature control is terminated when all of the set Wait OFF time has elapsed.</p>

4.2.4 Checking the Operation after Timer Setting

- In case Wait ON Timer is set
 - (1) After setting the Wait ON timer, press start.
 - (2) After the Wait ON Time, the heater operates to reach the setting temperature.
(If you set up the Wait OFF Timer, the Wait OFF Timer works automatically once the set temperature has reached.)

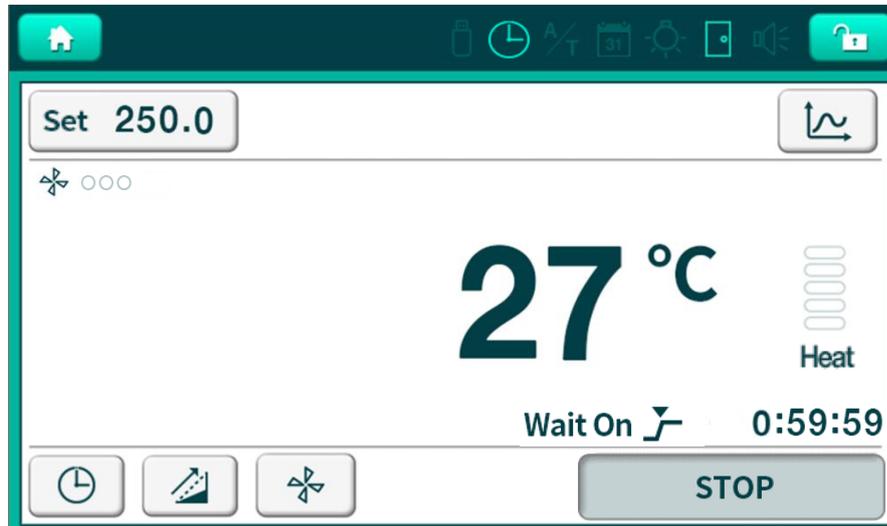

- In case Wait OFF Timer is set
 - (1) If you press the start button after setting the Wait OFF Timer, the instrument start the heating operation.
 - (2) The Wait OFF Timer starts once the target temperature has reached.
 - (3) Once the Wait OFF Timer reaches its input time, the instrument stops operation.

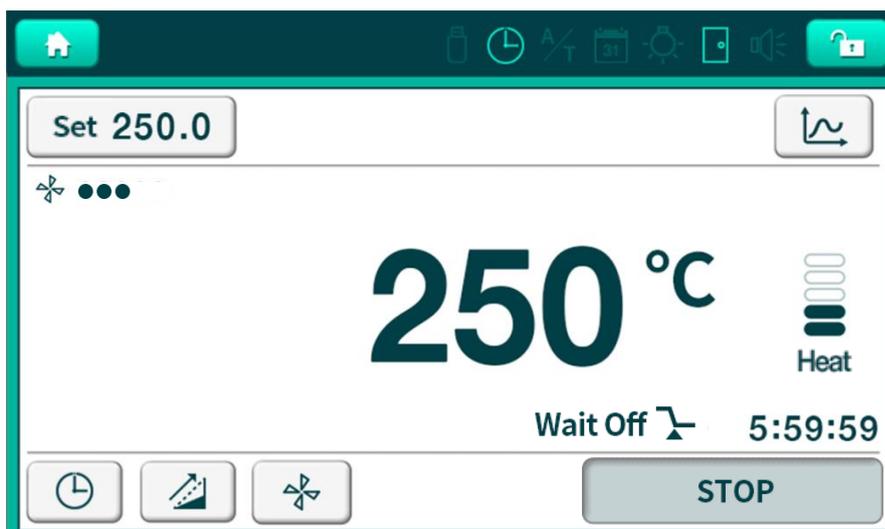

NOTICE

- If the Wait ON Timer and Wait OFF Timer are both set, the activated timer and the remaining time will only be shown in the display.
- If you press the start button when the instrument is not operating, the timer starts the temperature control according to the Wait On Timer/ Wait OFF Timer.
- If you set the Wait OFF Timer while the instrument is in operation, the new timer will be applied immediately without having to press the Start button again.
- If you want to change the Wait OFF timer during timer operation, you must turn off the Wait OFF Timer and reset the process.

4.2.5 Setting the Temperature Ramping Rate

Setting the temperature ramping rate is a function to protect samples or equipment from a sudden temperature rise.


4.2.5.1 Change the temperature ramping rate value setting

In 'System Settings > Temperature', the temperature ramping rate can be set in units of temperature increase rate per minute ($^{\circ}\text{C}/\text{min}$). The input range of the temperature ramping rate is from 0 to $50^{\circ}\text{C}/\text{min}$. [4.5.1 Refer to the temperature]


4.2.5.2 How to use the temperature ramping rate function.

Select the temperature ramping rate function, and press the start button.

- (1) When you press the button, the temperature ramping rate value set in System Settings > Temperature appears with an icon at the bottom left.

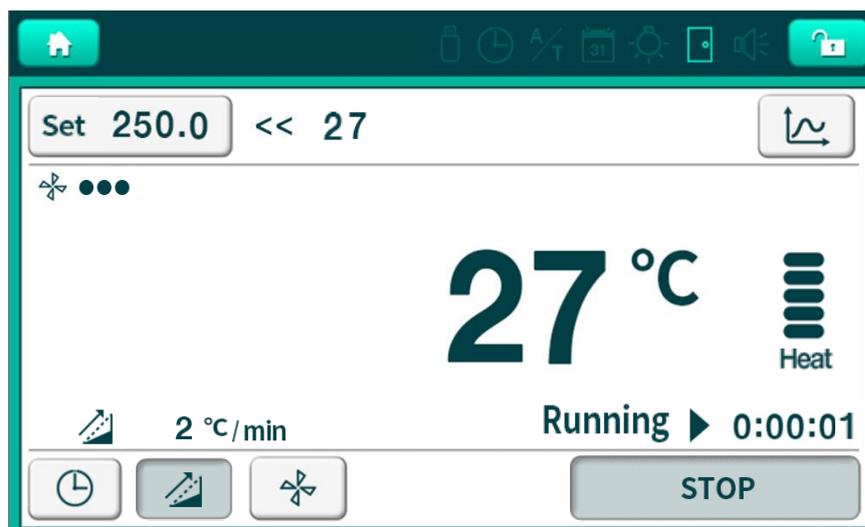

- (2) Once you press the start button, the heating operation will be started, and you will see the temperature ramping rate is being applied in real time at the top left.

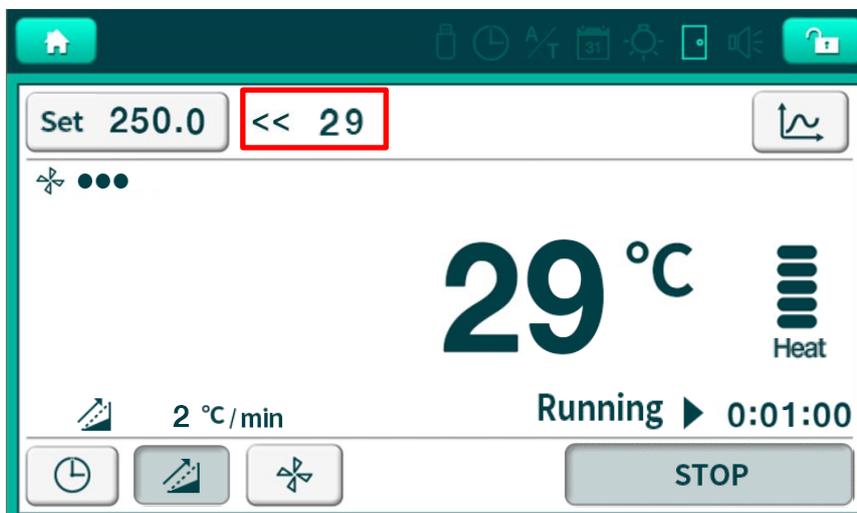

NOTICE


- The input range of the temperature ramping rate is from 0 to 50°C/min. But the temperature ramping rate may have a different maximum value for each model. Even if the input temperature ramping rate is greater than the maximum value, the temperature ramping rate could be operated with the maximum value that can be operated by the instrument.

	OF4-03P(W)	OF4-05P(W)	OF4-10P(W)	OF4-15P(W)
Temp ramping rate (°C/min)	0~13	0~9	0~6	0~5

- If the temperature ramping rate is set to 0°C/min and the temperature ramping rate function is used, the temperature ramping rate will run at the maximum value that the machine can output, not 0°C/min.
- For stable temperature control, please select the temperature ramping rate function firstly and then press the start button. Conversely, if the temperature ramping rate function is used while the device is operating, a temporary rapid temperature rise may occur, but control starts soon following the set temperature ramping rate.

4.2.6 Fan Speed Settings


You can set the fan speed by pressing the button,  in the Basic Mode.

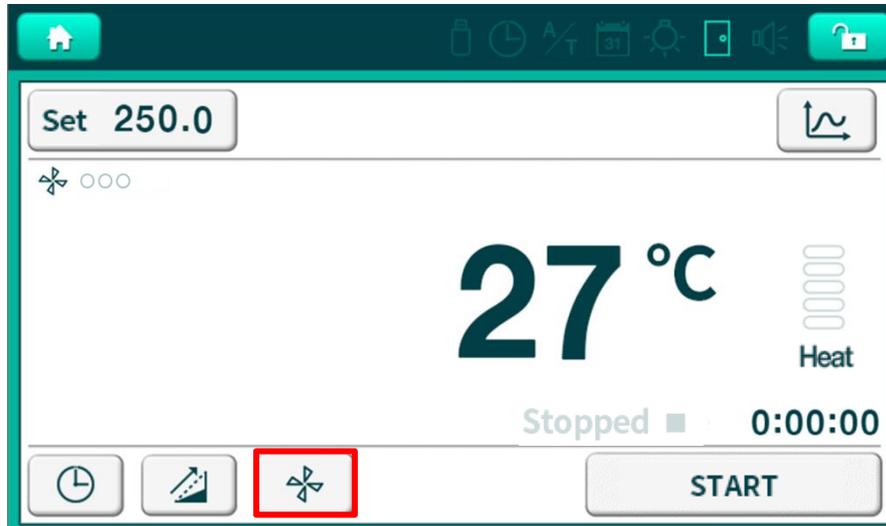

The fan speed can be set from stage 1, stage 2, and stage 3 according to the characteristics of the sample.



Once the fan speed stage has set and the start button has pressed, the screen returns to the basic mode, and then the set speed will be shown on the top left.

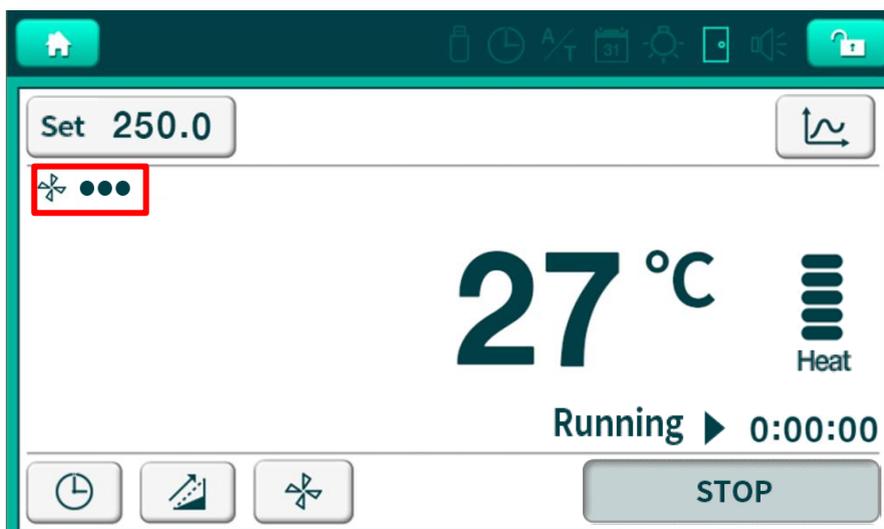

NOTICE

- When powder is dried, powder does not fly, and in order to have a temperature distribution similar to that of natural convection oven, an experiment was conducted using calcium carbonate.
- For the calcium carbonate used in the test, two different sizes were used: 5um or less and 44um or less.
- As a result of the experiment, we divided the fan speed into three categories as shown below.

Fan speed	Stage	Temperature Distribution	Powder blown
	1	Poor	Poor
	2	Fair	Fair
	3	Good	Good

- In general experiments, 3 stages of fan speed are recommended, and 2 stages are recommended when drying powder. Use step 1 only if powder is blowing despite setting to step 2.

⚠ CAUTION



- If the fan speed is lowered, the temperature performance such as Fluctuation and Variation may be deteriorated.

 **WARNING**




- Do not put flammable dust inside the instrument. If combustible dust enters the heater, it may cause a fire or explosion. This device is not an explosion-proof structure.



- Do not place explosive, flammable, flammable, or oxidative chemicals such as alcohol, benzene, gasoline on top of the device, store them, or put them in the instrument and operate them. There is a risk of fire. This device is not an explosion-proof structure.


4.2.7 Real Time Graph

The graph will be displayed, once you click the icon  on the top right. If the oven is not running, the event and graph buttons will be inactive.

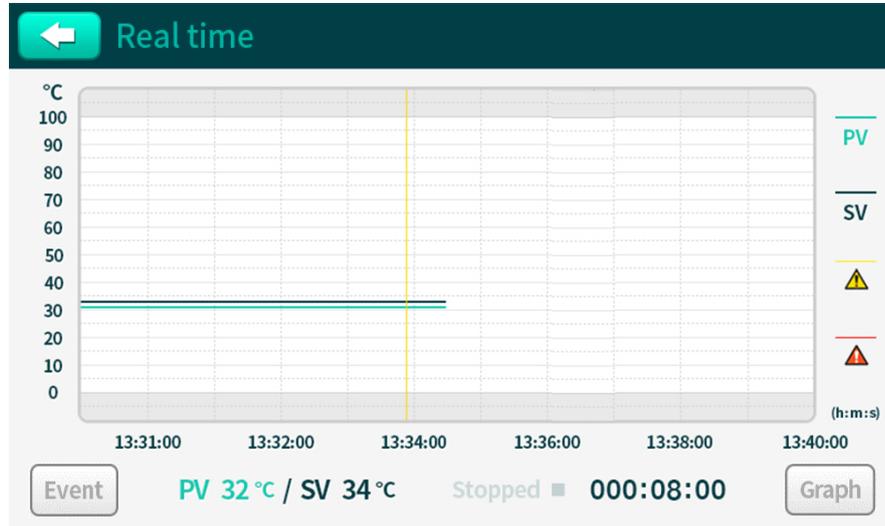


Once you turn on the oven, the event button and graph button will be activated, and event/warning, PV/SV will be shown at the same time.

The display will be moved once you click the event button or graph button. Please refer to [4.4.7 Event] for more details.

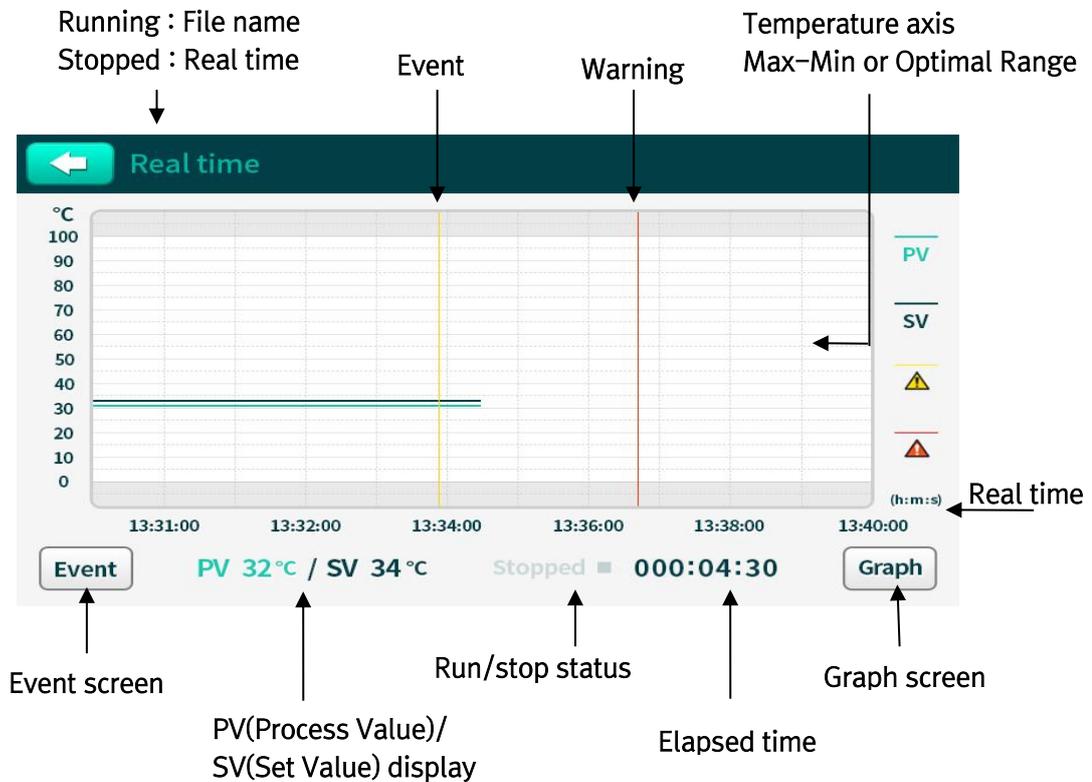

Once you go to the graph screen, you will see the following screen.

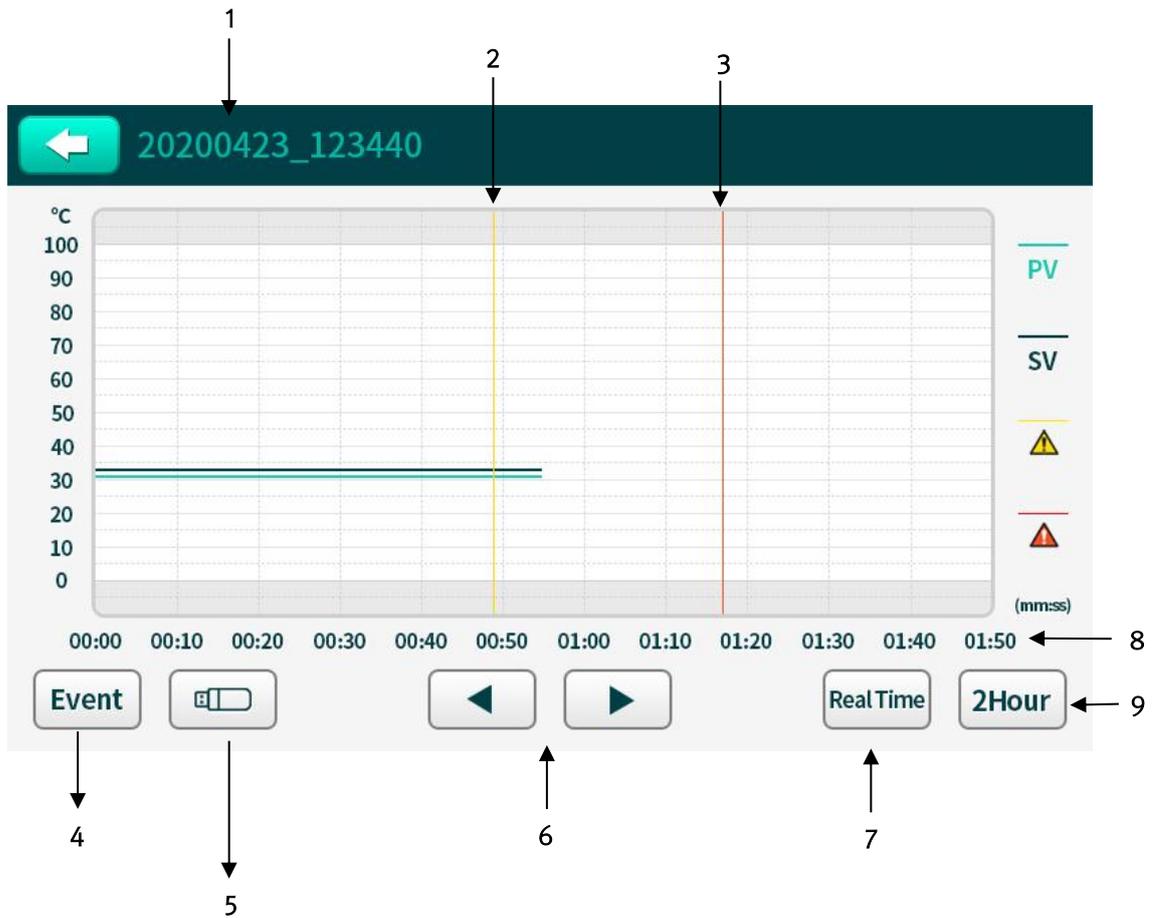

1	File name	The file name currently in progress will be displayed.
2	Event	The event data will be recorded they are occurred.
3	Warning	The warning data will be recorded they are occurred.
4	Event	Moves to the event/alarm view screen that occurred within the current file.
5	USB	Save the current file to USB.
6	Displaying graphs	Move the data screens left and right within the graph.
7	Real time	The screen will display the real time graph.
8	selecting time axis	You can select the time axis for 2 hours → 6 hours → 12 hours → 1 day → 1 week → 1 month.
9	elapsed time	The elapsed time will be shown in hours: minute format.

4.2.8 USB Storage function

The OF4 series can automatically save up to 54 files for 1 month if the power is not turned off in the internal memory. There are 54 file limits in the internal memory and the oldest data will be deleted first. Please use the USB drive for safe storage.

There are three ways to use the USB storage function, and the methods are as follows.

Division	How to use the USB storage function
How to save completed experiment data before USB connection	After connecting USB, you can save it in General Settings → Data. [4.4.6 Refer to Data]
How to save data when connected to USB while the device is running	After the end of the experiment, you can save it in General Settings → Data or press  the button in the real-time graph to save it. If the save button is pressed before the end of the experiment, only the data until the save button is pressed are saved.
How to save data after USB connection	If a USB connection is made before pressing the start button, it is automatically saved to the USB.

CAUTION

The internal memory creation limit is 54 files, and the storage is about 1 month. Since it is not automatically saved when connected to USB while the device is running, it must be saved in General Settings → Data or by pressing  the button in the real-time graph.

WARNING

If the creation limit is exceeded, the oldest files are deleted first, and when the power is turned off, all internal memory is deleted. Please use the USB drive for safe storage.

The data storage Popup is as follows.

<p style="text-align: center;">Notice</p> <p style="text-align: center;">Out of internal memory error.</p> <p style="text-align: center;">Acknowledge</p>	<p style="text-align: center;">Notice</p> <p style="text-align: center;">The internal memory is not ready.</p> <p style="text-align: center;">Acknowledge</p>
<p style="text-align: center;">Lack of storage in the internal memory.</p>	<p style="text-align: center;">Unknown error related to the connection to the internal memory</p>
<p style="text-align: center;">Notice</p> <p style="text-align: center;">USB is being connected. This message automatically disappears when USB is connected.</p> <p style="text-align: center;">Acknowledge</p>	<p style="text-align: center;">Notice</p> <p style="text-align: center;">USB memory is full.</p> <p style="text-align: center;">Acknowledge</p>
<p style="text-align: center;">Connecting to the USB drive</p>	<p style="text-align: center;">Lack of storage in USB drive</p>
<p style="text-align: center;">Notice</p> <p style="text-align: center;">USB flash drive is not supported format.</p> <p style="text-align: center;">Acknowledge</p>	<p style="text-align: center;">Notice</p> <p style="text-align: center;">USB flash drive is not supported format. (The device supports only FAT32)</p> <p style="text-align: center;">Acknowledge</p>
<p style="text-align: center;">Unknown error related to the USB connection</p>	<p style="text-align: center;">Improper format for the USB</p>
<p style="text-align: center;">Notice</p> <p style="text-align: center;">USB device not recognized. Try again in a few minutes.</p> <p style="text-align: center;">Acknowledge</p>	<p style="text-align: center;">Notice</p> <p style="text-align: center;">Data saving is complete.</p> <p style="text-align: center;">Acknowledge</p>
<p style="text-align: center;">USB is not found</p>	<p style="text-align: center;">Completed saving to the USB drive</p>

4.2.9 Instantaneous Outage Recovery Features

If the power is restored within 30 seconds of an instantaneous power outage, please follow the following procedure.

Before the Instantaneous Outage	Operation after Recovery from Instantaneous Outage in Basic Mode Control
Stopped	Stop
Running	Run
Wait ON Timer is On	The elapsed Wait ON Timer time is restored and the Wait ON Timer is started.
Wait OFF Timer is On	The elapsed Wait OFF Timer time is restored and the Wait OFF Timer is started.


Before the Instantaneous Outage	Operation after Recovery from Instantaneous Outage in Program Mode Control
Stationary	Stop
In operation	Restart the operation after recovering the process step, elapsed time and repeating cycle. If the process step is not yet started, it restarts from the beginning.
In case temperature/ timer limit is set	Proceed the current step after releasing the temperature/ time limit.
Maintaining by the maintain button	Release the maintaining function and proceed the step.
In case the temperature is maintained by the function in Closure Mode	Proceed the operation by keeping the maintaining the status.

4.3 Program Mode

In Program Mode, you can control the temperature and time for each step through the program No.1 through No.10, and sets the number of repetition and shutdown function. If you press the



button at home, the screen will switch to the Program Mode

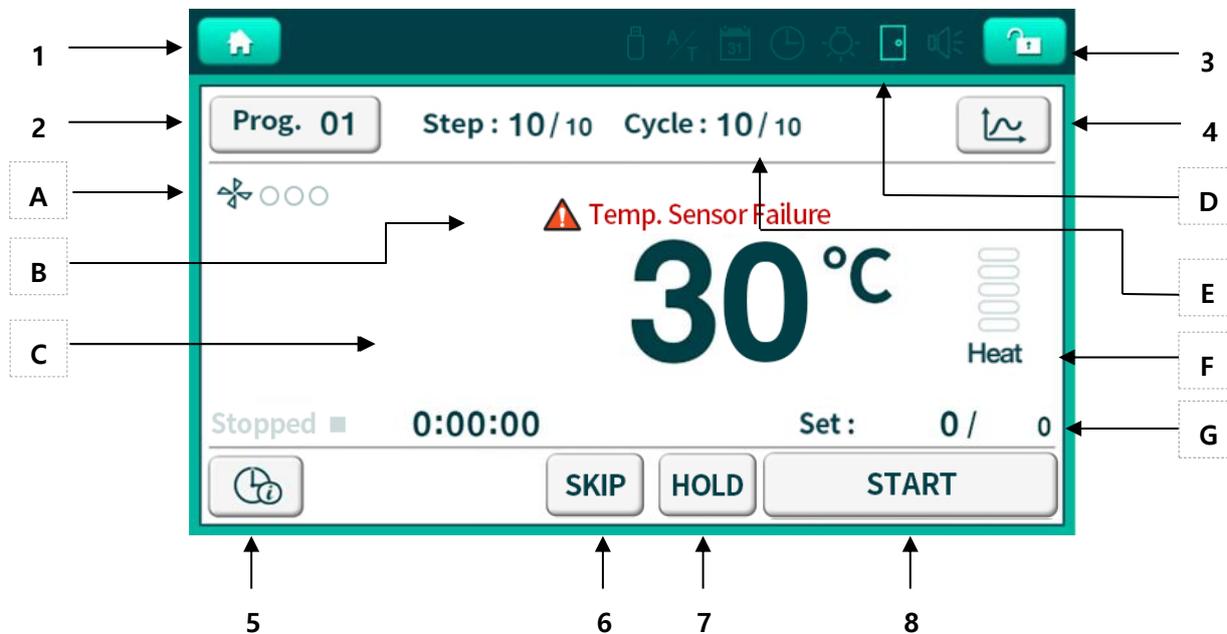

[Display of Program Mode]

(1) Status Display

A	Fan	Displays the set speed among the five stages of the fan's speed.
B	Warnings	When a warning occurs, an alarm sign appears, and a pop-up notification window appears.
C	Current Temperature	Indicates the current temperature inside the chamber.
D	Operating Status	 Auto Tuning  Setting Timer  Door Open/ Close  Sound On/ Off  USB connection


		 USB not recognized  Data transfer via USB
E	Status Icon Step/ Repetition	Represents the current/ target step and repetition.
F	Heating amount	Displays current heating amount
G	Target Value	Real-time setting value/ Current step setting value are represented.


(2) Buttons

1		Switch the screen to home. To change modes (to switch between Basic Mode / Program Mode) General/ System Settings When the power is on, the last operated mode will be shown.
2		You can set the program mode's operation.
3		Screen Lock On/Off
4		You can move to Graph screen.
5		Program information: You can check the selected program's operation information
6		You can skip the current step while the program is in operation.
7		You can maintain the current step when the program is in operation.
8		It controls the temperature. The button will be changed to "Stop" button after starting the operation.

4.3.1 Operation and Stop in Program Mode

- (1) Press the button,  in the Program Mode.
- (2) Select the program number by press the arrow buttons in the setting window of Program Model. [Refer to 4.3.2 Setting Program Mode / 4.3.4 Program Operation Settings].

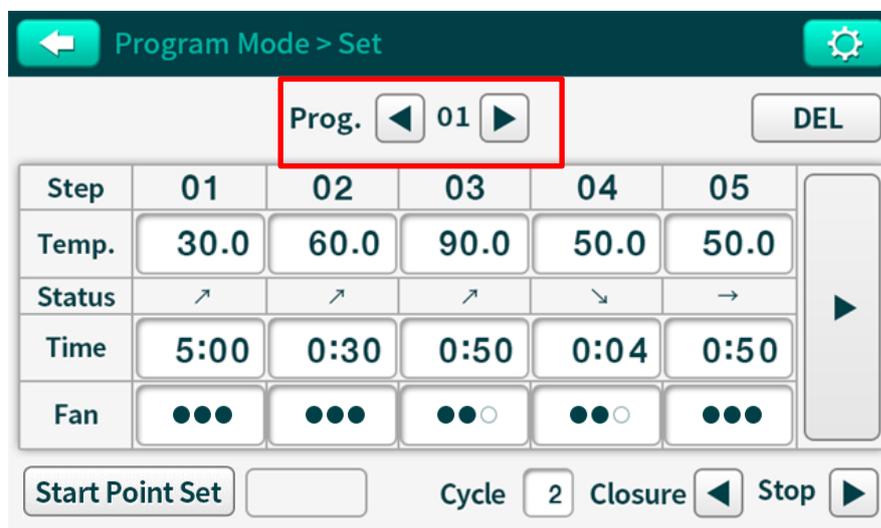


- (3) If you press the button, , after selecting the number of the desired program, you will be transferred to the operation mode display and the newly set up value will be applied.
- (4) Press the button, , to operate the selected program.
- (5) To terminate the operating program, press the button  in the operation display in the program mode.
- (6) If the last step of the program operation is completed, the instrument operates a program according to the set up value for the termination (maintain, p01~10, hold).

NOTICE

- Please check the temperature, step, and time value of the program setup display before the program.
- If you execute the program that has no step value, the instrument will sound an alarm and will not be operated.

4.3.2 Setting Program Mode

You can change and confirm the saved program information (program number, starting temperature, Fan speed, temperature time info of each process, cycle, closure).

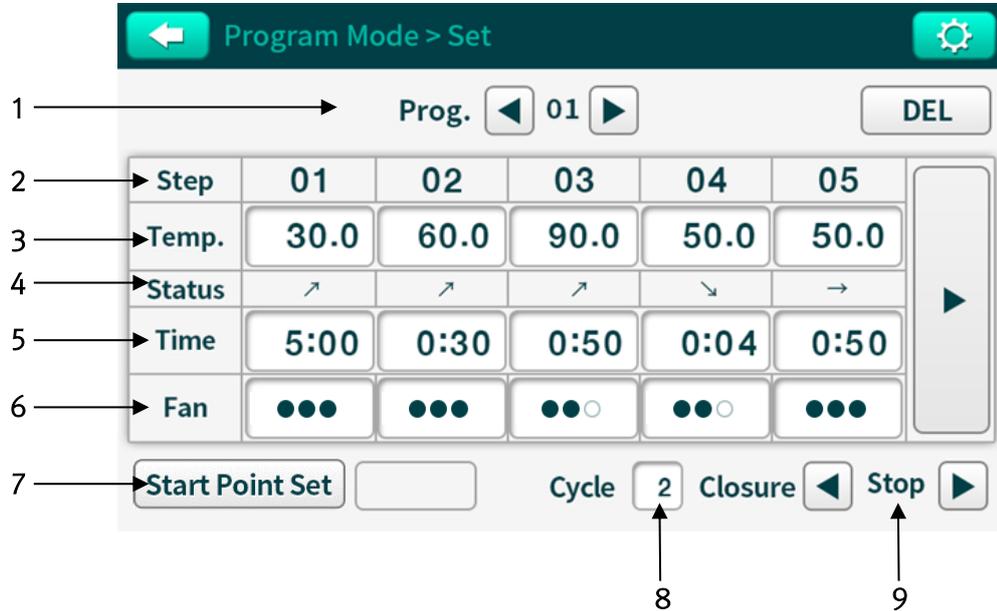

	Information	Description	Range of Input Value
1	Program	The maximum number of program model ten.	
2	Step	The maximum number of step in each program is 10. To set the steps greater than 06, please use arrow button.	
3	Temperature	A target temperature may be set in each step.	0~250
4	Status	The status diagram illustrates the increasing, maintaining, and decreasing states of the temperature.	
5	Time	Target time information of the operation can be set in each step.	00:00~99:59
6	Fan	You can set the Fan speed.	Step 1,3,5
7	Start Point Set	You can set the target temperature when the program starts.	0~250
8	Cycle	The number of cycle may be set in the range.	0~99
9	Closure	After completing the last step of the selected program, you may set the next operation.	Stop, Prog. 1~10, Continue

NOTICE


- If the set temperature of the Program Mode is not reached after activating the Wait On Timer, the first step of a program will not start.
- A program that continues after the previous program starts the first step immediately without converging to the set temperature.
- If you run a program that does not have a step value entered, an alarm sound will be ringing and the program will not run. • After you change the setting values for each program, press the arrow buttons (left and right) to automatically save the changed setting values.
- Press the delete button on the upper right corner to reset the values set for the program.

NOTICE

[Example of program entry]

If you enter the initial temperature value as 40°C and a value of steps 01 to 05 as shown in the table, the instrument controls the temperature as described in the graph below.


Steps	Initial Temp.	01	02	03	04	05
Temp. (°C)	40	100	100	150	150	250
Time		00:15	00:20	00:15	06:00	00:15

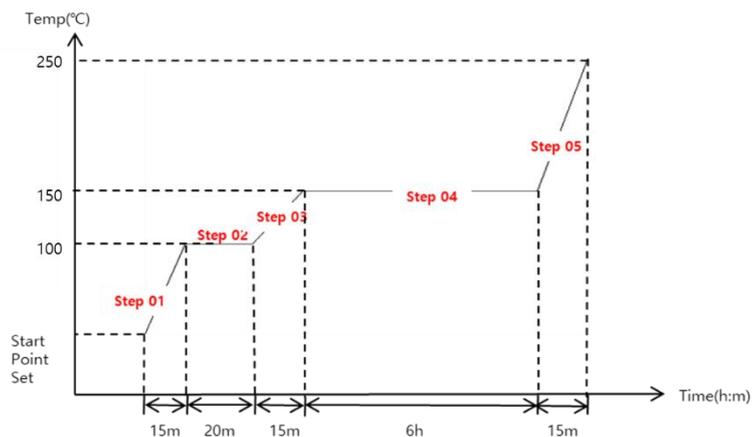

- External environment or lack of stage setup time can cause a time delay of the set temperature.
- At this point, the instrument extends the operating time of the current phase to directly advance to the next step or to meet the target temperature, in accordance with the permissible limit set in Program Mode > Function [Refer to 4.3.5 Tolerable Temperature and Tolerable Time].

4.3.3 Confirming the Information during the Operation

If you press the button  in the Program Mode, the screen will show you the information of the operating program.

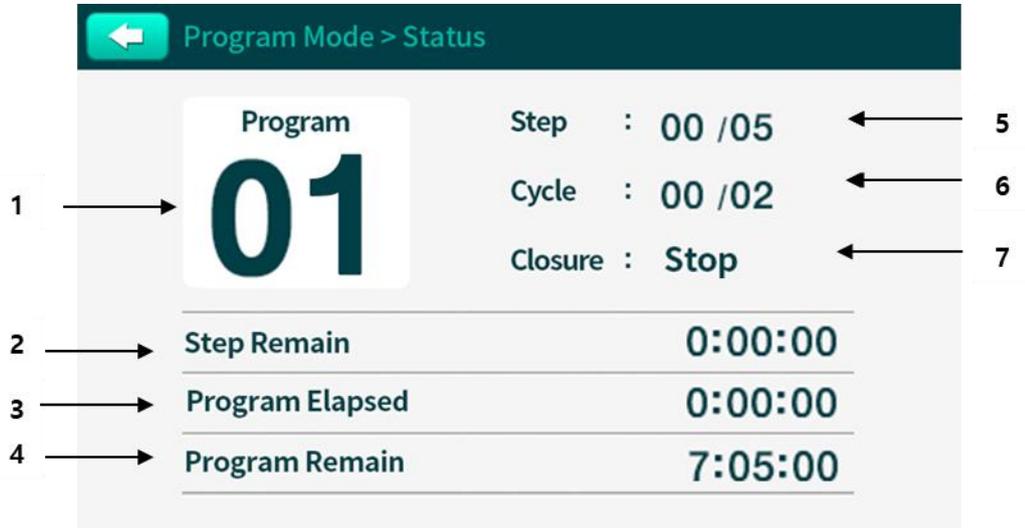

1	Program No.	Selected program number
2	Remaining time of the current processing step	Remaining time of the current processing step
3	Program Elapsed	Elapsed time of the selected program
4	Program Remain	Remaining time of all the steps of the program
5	Step	The current processing step/ the last step
6	Cycle	The repeating number of the current processing step/ the total number of repetition
7	Closure	The next processing step after completing the current program


4.3.4 Program Operation Settings

4.3.4.1 Start Point Set

"Start Point Set" is a feature that allows you to specify the initial temperature at which step 01 starts in the selected programs. If the target temperature is not reached, the program does not start.


If the "Start Point Set" is "off", the step 1 will start from the current temperature, and it will be raised to the target value during the "step 1" processing time.

- How to "Start Point Set"

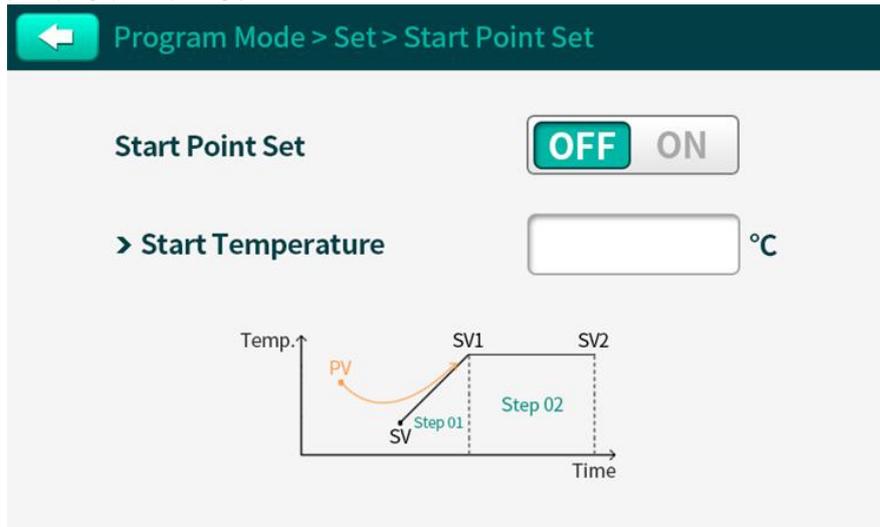


[PV: Process Value, SV: Set Value]

- (1) Go to the menu, Program Mode> Set> and click the "Start Point Set" button. Change the value from "OFF" to "ON" of the Start Point Set function

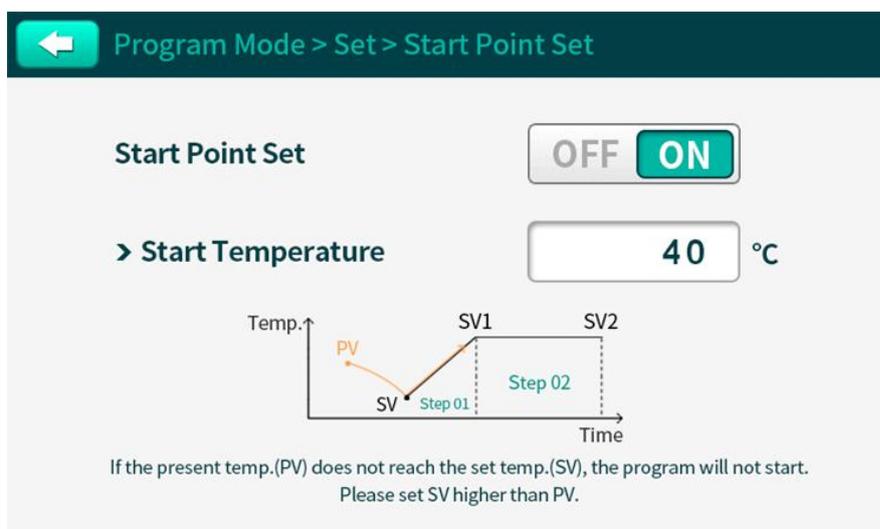

- (2) Activate the Start Point Set function and enter the desired start temperature value. (However, the program will not start if the target value of the start temperature is not reached.)

(3) Press the  button to complete the setting process.

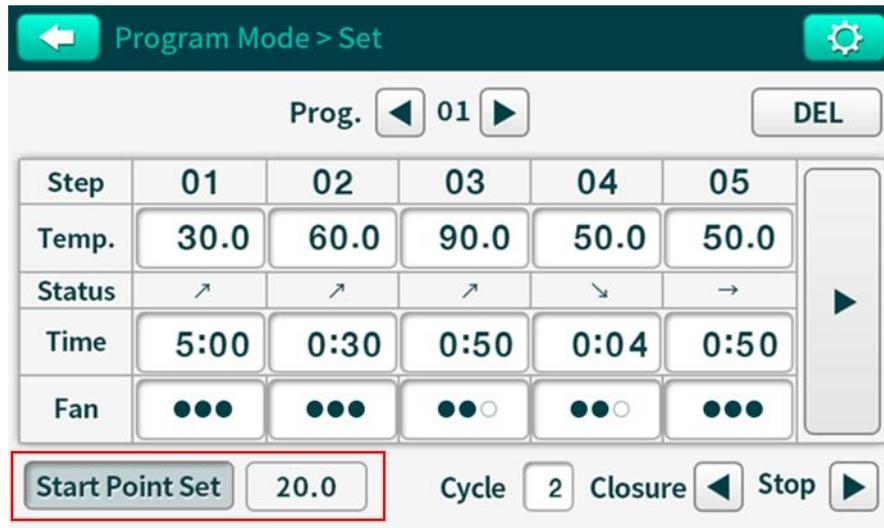


NOTICE

- The start temperature of the "Start Point Set" function should be set higher than the current temperature. The program will not start if the temperature does not reach the set start temperature.

4.3.4.2 Setting the number of cycles and closure

The function either repeats a program that you have set up, maintaining the final step, or proceed the next programs.

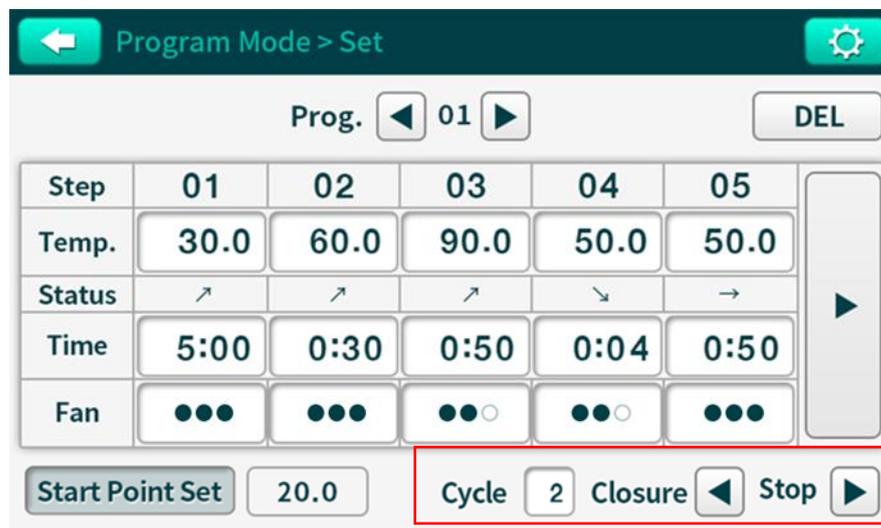

Cycle	The input range of the cycle is from 0 to 99.	
Closure	After completing the final step, you can select among the three operations shown in the table.	
	Stop	Terminate the program control.
	p(program) 01 ~ 10	Continues the following selected program number.
	Hold	Maintain the target temperature that was set for the final step.


NOTICE

- The subsequent program begins from step 01 without reaching the target temperature [see 4.3.4.1 Start temperature].
- If you select the previously selected program number when setting the shutdown, the program repeats indefinitely.

4.3.4.3 Setting the Skip Retention Function

The Skip Retention Function skips the current step and executes the next step while not stopping the operating program.

In addition, even when you need to maintain the current step, you can easily maintain that step by utilizing the maintaining function without stopping the operating program.

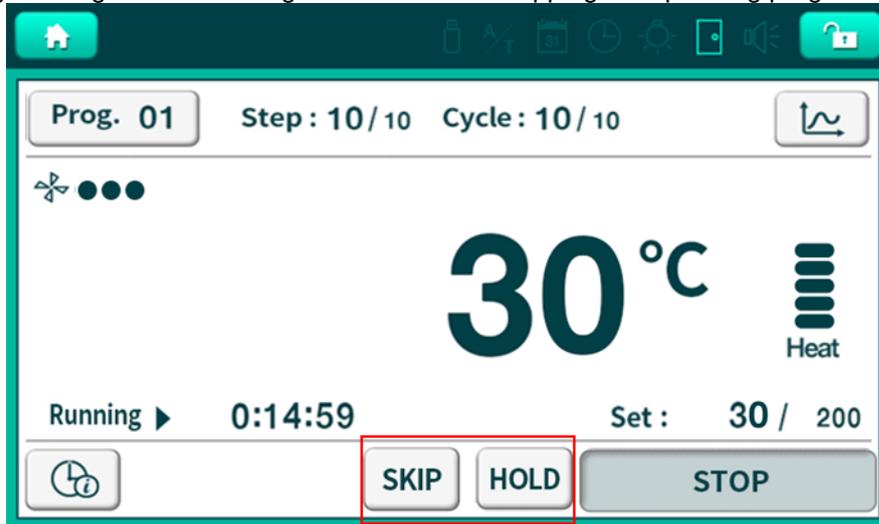


	Function	Operation
1	In case you press the SKIP button while the program is in operation	Proceed the next step after skipping the current step
2	In case you press the HOLD button while the program is in operation	Stop the current processing step and maintain the current temperature. If you press the button one more time, it releases the maintaining function.
3	In case you press the SKIP button when HOLD is activated.	The instrument stops the current processing step, and proceed the next step.
4	In case you press the SKIP button at the final step.	The instrument terminates all the program. (Stop the operation)

4.3.5 Tolerable Temperature and Tolerable Time

The Permissible Temperature and Time Limit feature assumes certain range of errors to be normal even if the target temperature or time is not reached. If you press the  button in the program setting window, the screen switches to Program Mode> Function.

You can set the permissible temperature and time limit. Please click  icon on the upper right corner for the information about the tolerable temperature and tolerable time.

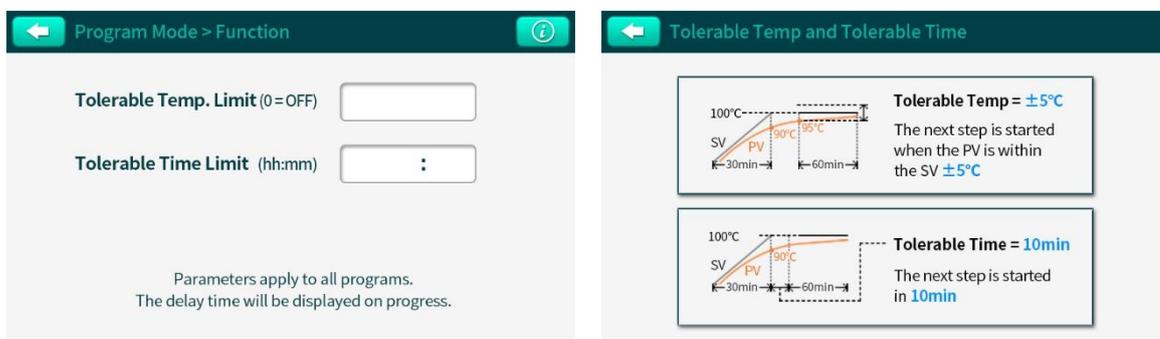

Tolerable Temperature Limit	<p>When controlling the temperature, you can set the tolerance of the set temperature and the actual temperature when the target temperature has not been reached for the time set in the current step. If the temperature is within the temperature limit error range (set temperature - tolerance) and the tolerable time limit is zero, it considers the set temperature to be reached and proceed to the next step.</p> <p>Factory default is set to 0°C (OFF).</p>
Tolerable Time Limit	<p>When controlling the temperature, you can set the maximum waiting time for the current step in case the target temperature is not reached in the target time that you set for the current step.</p> <p>If the set temperature is reached before the time limit, the instrument proceeds immediately to the next step. In case the set time + tolerable time exceeds, the instrument proceeds the next step even if the target temperature is not reached. For example, your target temperature is 100°C and the target time is one hour and the tolerable waiting time is set for 10 minutes. If the temperature is</p> <p>Factory default is set to 00:00.</p>

Setting the tolerable temperature and the tolerable time limit is describe as below.

- (1) Change the tolerable temperature and tolerable time limit.
- (2) Press the button,  to save the input value and switch to the program setting display.

NOTICE

The changed value of a program will be applied to each step of the program.


- If the tolerable time is not set, the controller waits for the current temperature to enter the tolerable temperature range without proceeding the next step.
- If the tolerable time is set, it proceeds the next step after the tolerable time passed, even if the current temperature does not enter the tolerable temperature range.

[Example of entering the program function]

(1) In case you entered the tolerable temperature limit as shown below. (Tolerable time limit = 0)

Initial Temperature (°C)	Temperature of Step 1 (°C)	Time of Step 1 (min)	Tolerable Temperature (°C)
30	50	30	2


If the target temperature of 50°C is not reached within 30 minutes of program step 1, the next step will proceed when the [Set temperature - Allow temperature value of 48°C is reached.

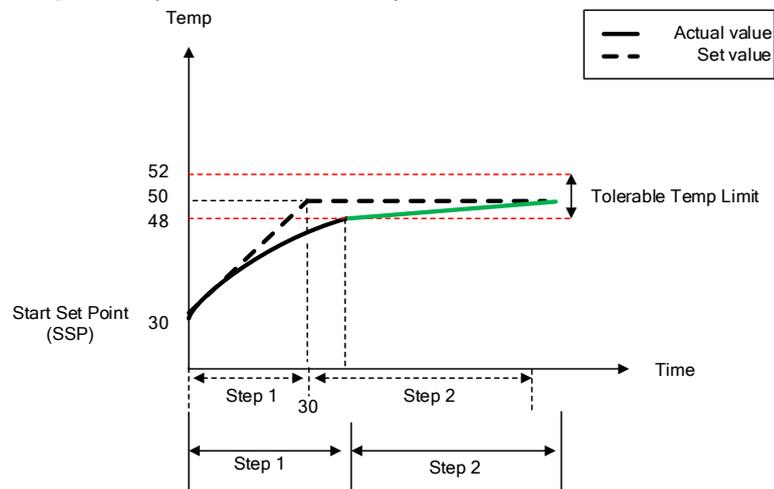

(2) In case you entered the tolerable time limit as shown below.

Initial Temperature (°C)	Temperature of Step 1 (°C)	Time of Step 1 (min)	Tolerable Time (min)
30	50	30	5


If the set temperature of 50°C is not reached within the setup time of program step within 30 minutes it elapsed time (set time + allowed time) reaches 35 minutes the next step will proceed.

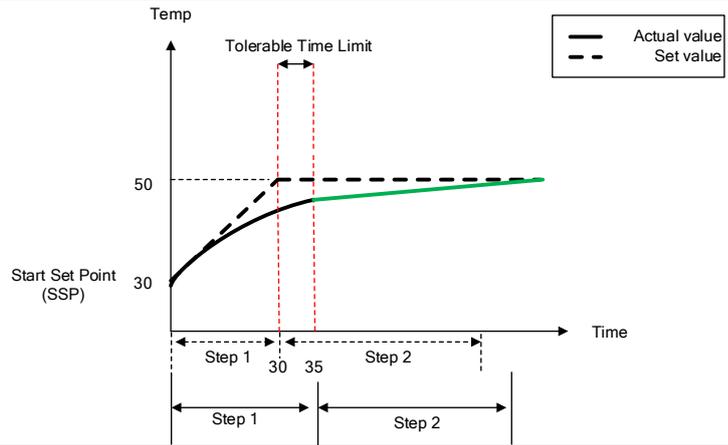

4.4 General Settings


In General Settings, you can check and change the settings for Sound & Display, Clock, Language, Auto Run & Safety Lock Door, Data, Event, Communication.

Pressing the General Settings  button in the home screen takes you to the General Settings.

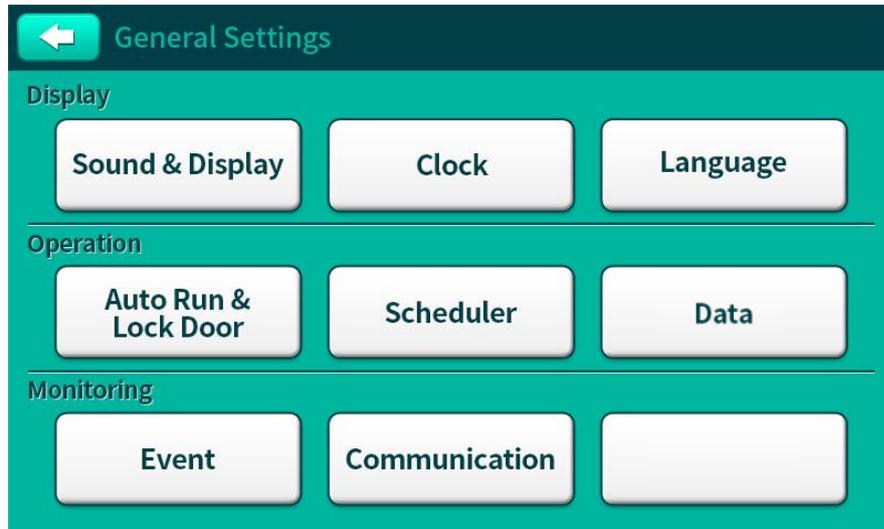

4.4.1 Sound & Display

In Sound & Display, you can set the sound generated when the screen is touched, on lamp by door and the Display Auto Dim function.

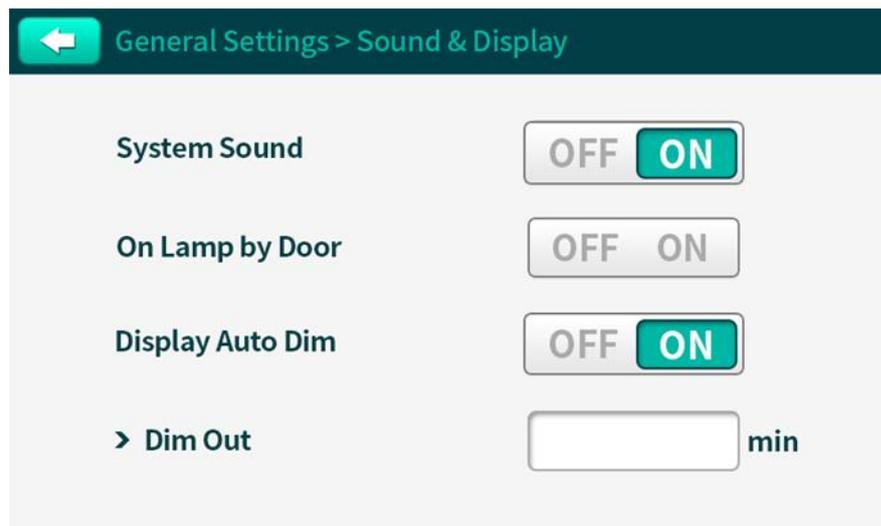

Item	Function	Input Value	Default
Sound Settings	Set the System Sound (touch screen sound). Even if it is set to OFF, an alarm sound occurs.	Off / On	ON
Display Auto Dim	Set the display Auto Dim function. If the touch screen is not touched for the entered time, the display turns off automatically.	Off / On	ON
Dim Out	Set the time for the display to turn off automatically.	0 ~ 30min	1

NOTICE

- OF4 Series does not support the on lamp by door.

4.4.2 Clock

The Clock is a function that sets the time within the device. The time set in the Clock is the standard for the date and time of the event recording [4.4.7 Refers to Event].

The screenshot shows the 'General Settings > Clock' screen. It features a keypad for setting the date and time. The date is set to 2020 year, 09 month, and 24 day. The time is set to Thursday, 00 hour, and 00 min. There are navigation arrows and a 'Save' button.

- (1) Choose an input field that you want to change among year, month, day, hour and minute.
- (2) You can enter the value when the keypad window pops up.

(3) You can select the day of the week with the left and right arrow buttons.

(4) Press the  button to save the changed value.

NOTICE

- If you press  button before saving, it cancels the changes and returns to the previous screen.


CAUTION



- The date (year/month/day) and time (hour, minutes) set in Settings > Clock may have discrepancies due to the characteristics of the components used in the controller. If the time needs to be measured precisely, this discrepancy can have significant effects. Users should fully understand these characteristics of this product. If necessary, consider periodic time synchronization actions as indicated in Section 5.1 Inspection Cycle Guidance, or consider using another product with more precise time adjustment functions in conjunction with this product.


4.4.3 Language

You can set the default language that appears on the device. The default language is Korean, and you can choose among Korean/English/Chinese (Chinese will be supported later).

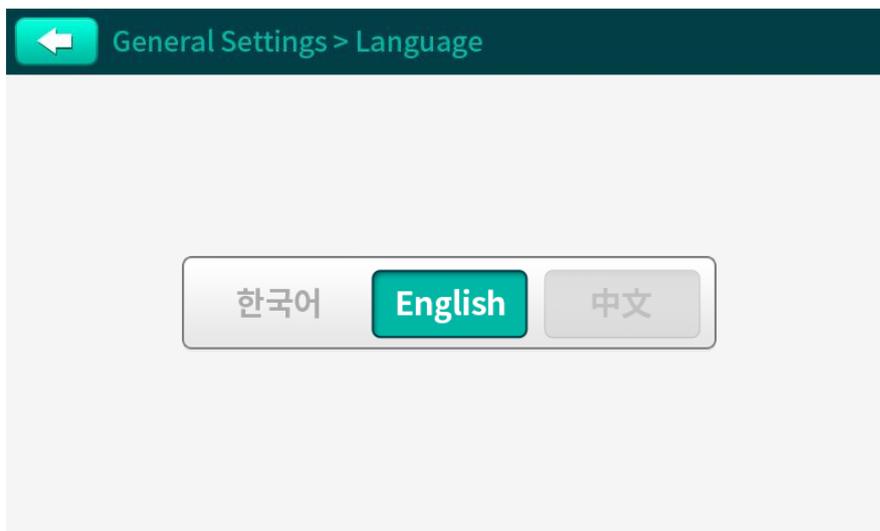

4.4.4 Auto Run & Door Lock

When power is turned off and restored after more than 30 seconds, Auto Run function makes the user set the function to determine whether or not to operate by remembering the state before the power turns off.

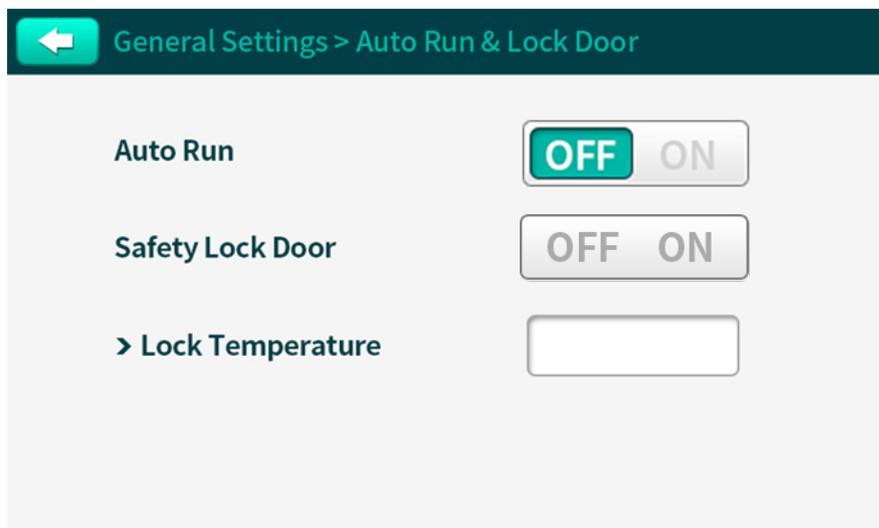

Item	Function	Input Value	Default
Auto Run	When the power is turned off for more than 30 seconds during temperature control and restarts, set the function to automatically run at the previously set temperature.	Off / On	OFF

NOTICE

If the user sets the Auto Run and the power is restored after the device is turned off for 30 seconds or more during temperature control, follow the procedure below.


Previous States	Operation in Basic Control	
	Auto Run Off	Auto Run On
Stopped	Stop	Stop
Running	Stop	Operation
Wait ON Timer	Stop	The elapsed time of the Wait ON Timer is not be restored and returns to the initial setting.
Wait OFF Timer	Stop	The elapsed time of the Wait OFF Timer is not restored, and starts from the beginning.

※ Refer to [4.2.9 Instantaneous Power Failure Recovery Function] for operation by instantaneous power failure (recovery before 30 seconds).

※ Safety Lock Door function is not embedded in the OF4 Series.

4.4.5 Scheduler

This is a function that executes the set program number according to the start time of the set day of the week. This function can be used only in models that support the Program Mode. **(OFF is the default setting for the scheduler. However, even if the scheduler is turned on, the scheduler will not work if the day of the week is not selected.)**

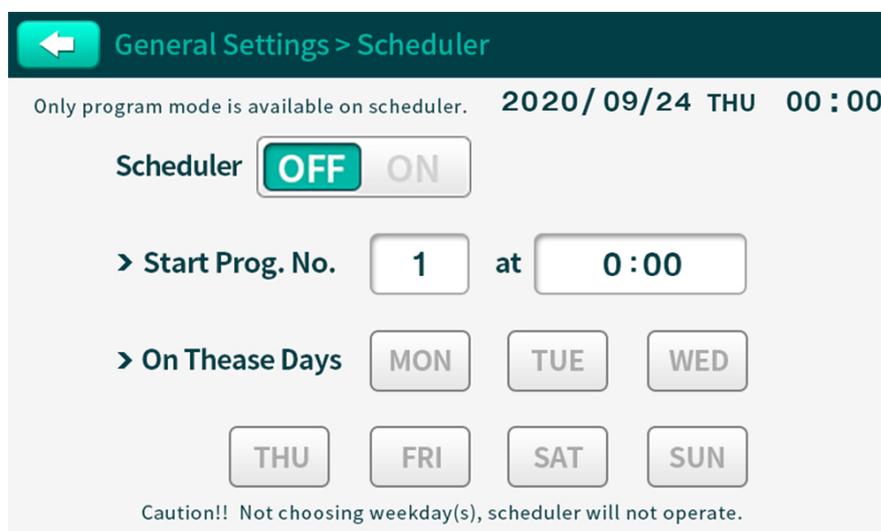


Item	Function	Input Value	Default
Start Program Number	After setting the Program mode, enter the desired program number.	01~10	1
Time	Program Mode can be set to start at the desired time.	00:00~24:00	0:00
Select the Day of the Week	You can select the day of the week you want to operate. Once you select the day, highlighting will be activated.	Month~Day	-

NOTICE

- When the scheduler is reserved (ON), the scheduler icon  is displayed on the main screen.
- For running products, the scheduler function is not executed even if the scheduler is set.
- If the corresponding program cannot be executed due to an error at the time of execution, the function is not performed.
- The scheduler will not operate without the “day” being selected, even though the scheduler is reserved (ON).

4.4.6 Data

You can check the data stored in the internal memory. Data recorded in the internal memory is deleted when the power is turned off. When used without turning off the power, about 1 month, up to 54 files are saved. If there are more than 54 saved files, the oldest files are deleted first, so USB storage is recommended.

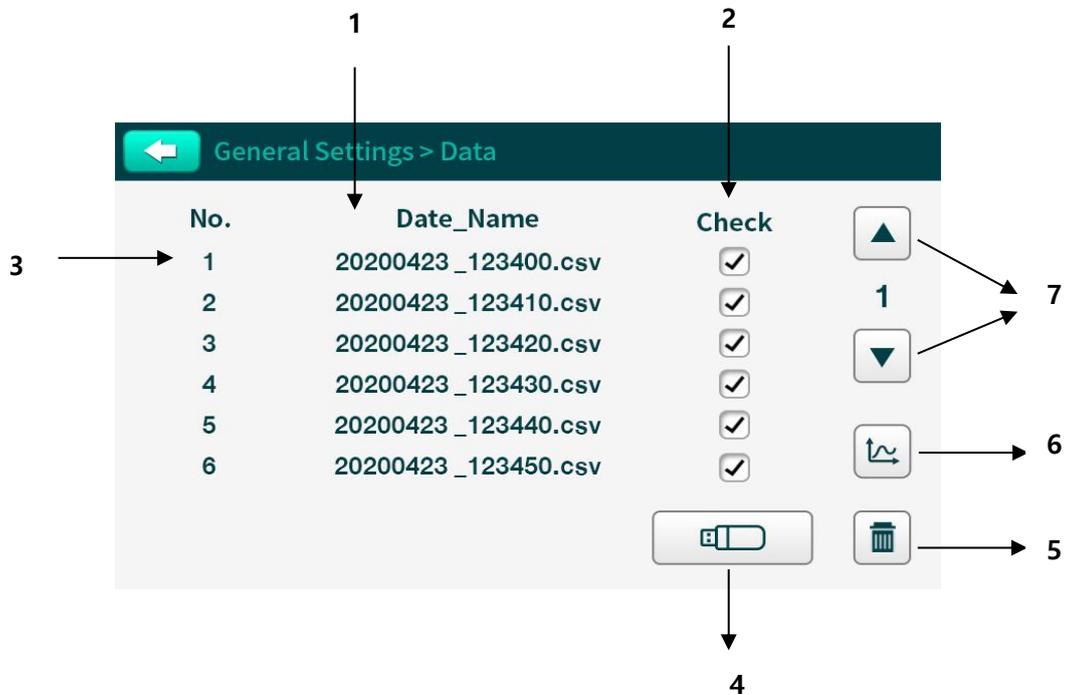

1	The file name is year, month, day, hour, minute, second. It is saved as a csv file.
2	After selection, you can move to the graph screen, save to USB, or delete it. Only one selection is possible to move the graph screen. You can select more than two USB storage and deletion options.
3	Up to 54 numbers are displayed.
4	Copies the selected files to USB. It is saved in the JEIO_DE folder. If there is no folder, it is automatically created and saved in CSV format.
5	Deletes the selected file.
6	The selected file is displayed on the graph screen. By checking the saved data through the graph screen, you can check the USB storage and file to be deleted.
7	You can select a page and move up to 9 pages.

The file format is saved in CSV format and can be opened as an Excel file. In Excel files, one decimal place is omitted for PV (Process Value), SV (Set Value), and MV (Manipulated Value).


When the power is turned off, all data in the internal memory is deleted. If the creation limit is exceeded, the oldest files are deleted first, and when the power is turned off, all internal memory is deleted. Please use the USB drive for safe storage.

	A	B	C	D	E	F	G	H	I	J	K	L	M	N	O	P
1	Model	4930	Option	48												
2																
3	Year	Month	Date	Hour	Minute	Second	Event	Temp Unit	PV	SV	MV	DO1	DO2	DI	OPT1	OPT2
4	20	12	27	2	18	57	0	0	196	270	0	49156	0	3	0	0
5	20	12	27	2	19	7	2	0	197	270	958	49164	0	3	0	0
6	20	12	27	2	19	17	0	0	200	270	853	49164	0	3	0	0
7																

1	Models and options for OF4.
2	It is a unit of temperature and is expressed as 0=°C, 1=°F.
3	PV (Process Value) represents the current temperature.
4	SV (Set Value) represents the set temperature.
5	MV (Manipulated Value) represents the control output value of the heater.
6	It is a contact input value and indicates the door limit value.
7	The year, month, day, hour, minute and second the data was recorded.
8	It is the event number, please refer to 4.4.7 Event for the number details.
9	It is a contact output value, DO1 is the heater output, and DO2 is the circulation fan output value.
10	It indicates the preliminary value and indicates the preliminary DO and DI values.

4.4.7 Event

Event is the function to indicate the start of control and errors occurred in the device.

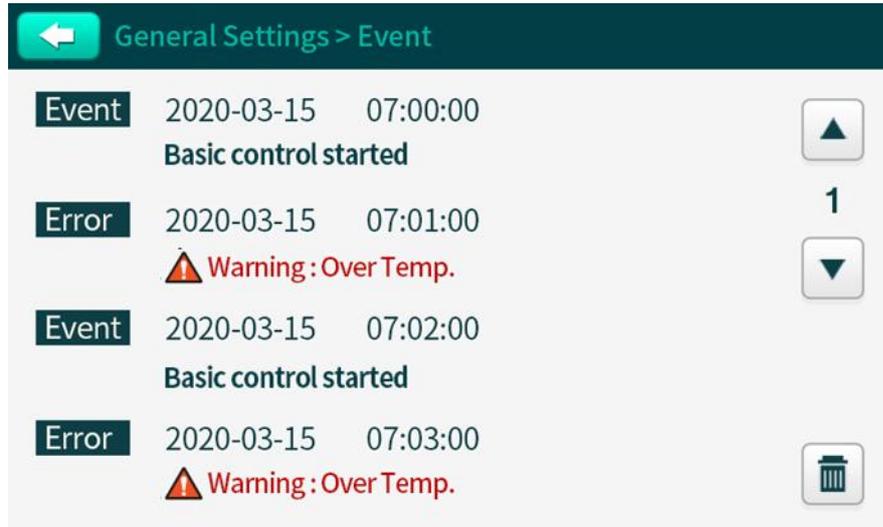

The latest event occurrence and time are displayed. Up to 4 events can be displayed on one screen, and you can move up to 9 pages by arrows. It can record up to 36 events.

Pressing the  button clears all the recorded events.


Event No.	Event	Remark
1	Door Lock Failure	N/A
2	High Temp. Deviation	
3	Low Temp. Deviation	
4	Over Temp.	
5	Temp. Rise Delay	
6	RJC Failure	N/A
7	Door: Open time exceeded	
8	High temp	
9	Sensor2 Failure	N/A
10	Temp. Sensor Failure	
11	Power Failure	
12	Board Failure	
13	Door:Opened	
14	Program started by Scheduler	
15	Basic control started	
16	Program control started	
17	Basic control completed	
18	Program control completed	
19	Auto Tuning started	
20	Auto Tuning completed	
21	Electric Panel Over temp	N/A

⚠ WARNING

- If there are more than 36 event records, they are automatically deleted sequentially from the oldest.
- Click the "Delete" button to delete all existing records of the Event History.
- When using USB, event records and experimental data are saved. Therefore, the use of USB is recommended.

4.4.8 Communication

It is the function that allows communication settings with LC-GreenBox (Option).

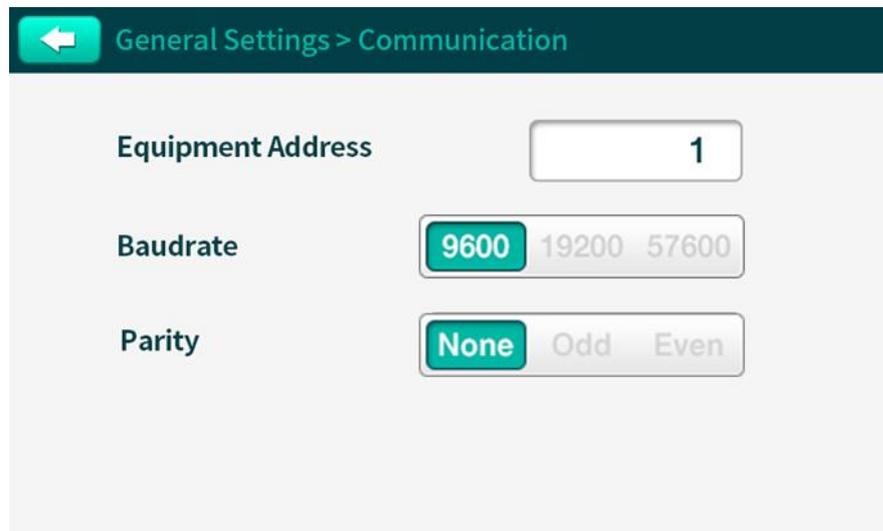

Item	Function	Input Value	Default
Equipment Address	Set communication Address.	1~255	1
Baud Rate	Set Communication Rate.	9600,19200,57600	9600
Parity	Set Communication Parity.	None, Odd, Even	None

NOTICE

- To connect JEIOTECH software and OF4 equipment, enter the same Port number (ex. COM3) on the computer screen [8.2 refer to the Connecting the software to the instrument]
- When using the LC-GreenBox, the Equipment Number must be set to the same number (1~4) you want to connect to the LC-GreenBox. Set the Baud Rate 9600 and Parity None.

(Check the user manual of LC-GreenBox for more information.)

4.5 System Settings


In the System Settings, you can check and change the settings for Temperature Input, Calibration, Auto Tuning, Alarm, Password, and Factory Default.

- (1) If you press the System Settings  button on home screen, the password window appears.




The image shows a password entry window titled "Enter Password (0 ~ 9999)". It features a large empty text input field at the top left. To the right of the input field is an "ESC" button. Below the input field is a numeric keypad with buttons for digits 1 through 9, 0, and a decimal point. To the right of the numeric keypad are three buttons: "Clear", a left-pointing arrow, and "Enter".

- (2) After entering the set password, press the Enter button to go to the System Settings window.
※ The initial password is set to '0000'.

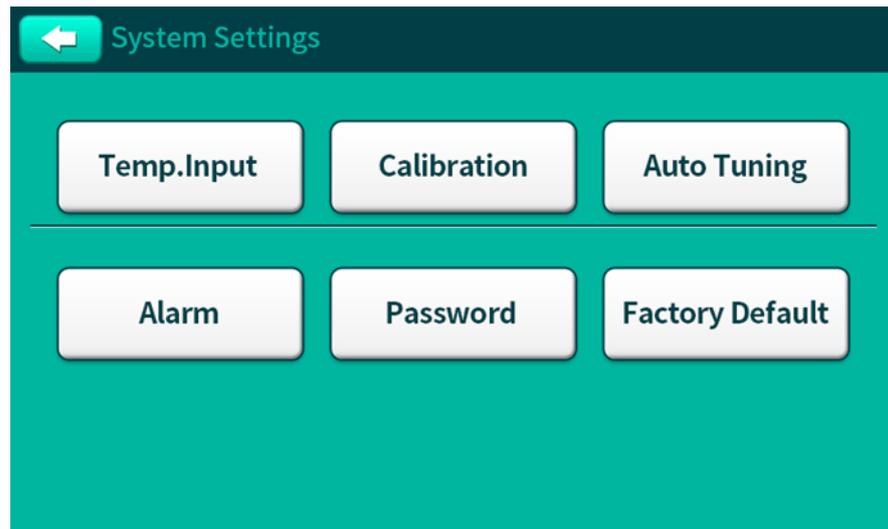

4.5.1 Temperature

Temperature & Temperature Ramping Rate can be set for the temperature unit and decimal point unit displayed on the screen. You can also enter the value of the ramping rate used in the basic mode.

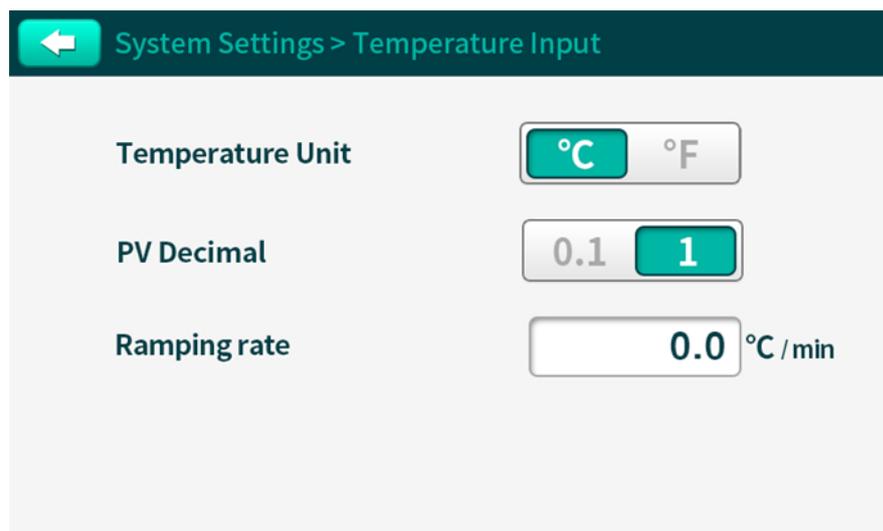

Item	Function	Input Value	Default
Temperature Unit	Set the unit of temperature.	°C / °F	°C
PV Decimal	Set the decimal place.	0.1 / 1	1
Ramping Rate	You can set the rate of temperature change that increases per minute. Click the temperature field to display a window where you can enter the temperature.	0~50°C	0

NOTICE


- If the temperature ramping rate is set to 0°C/min and the temperature ramping rate function is used, the temperature ramping rate will run at the maximum value that the machine can output, not 0°C/min.
 - Please refer to the 4.2.5 Setting the Temperature Ramping Rate the maximum output value for each device.
-

4.5.2 Calibration

When measuring the temperature inside the chamber by using the user's temperature sensor, if there is a temperature difference between the temperature sensor inside the device and the user's temperature sensor, you can calibrate the temperature sensor inside the device according to the user's temperature sensor. It is possible to calibrate temperatures accurately at up to three temperature points.

Actual Temperature		5.0 °C
	Uncalibrated	Calibrated
Temp 1	0.0 °C	0.0 °C
Temp 2	125.0 °C	125.0 °C
Temp 3	250.0 °C	250.0 °C

- (1) Specify Temperature 1, Temperature 2, and Temperature 3 to calibrate the temperature sensor inside the device and record them in the note (However, Temperature 1 < Temperature 2 < Temperature 3).
- (2) Go to the Basic Mode and set the set temperature as the Temperature 1 to be calibrated.
- (3) When the temperature converges to the set temperature and becomes stabilized, measure the internal temperature using the external temperature sensor and record it in the note.
- (4) Proceed with (2)~(3) by changing Temperature 1 to Temperature 2 and Temperature 3 and record the temperature measured by the external temperature sensor in the note.
- (5) You can go to System Setup> Calibration and enter Temperature 1, Temperature 2, and Temperature 3 in the Uncalibrated column. Also, enter the internal temperature measured by the external temperature sensor in the Calibrated column to complete the temperature calibration.

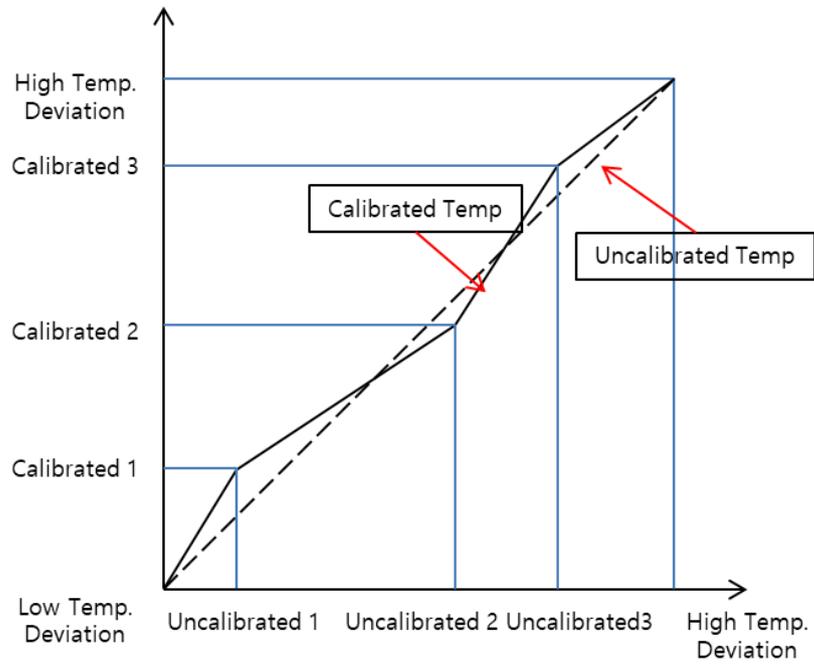


Item	Uncalibrated Input Value	Default
Temperature 1	-20~(Temperature2 -1)	0
Temperature 2	(Temperature1 +1) ~ (Temperature 3 -1)	125
Temperature 2	(Temperature2 +1) ~ 270	250

4.5.3 Auto Tuning

It is a function to update the PID control parameters for temperature control. Optimum temperature control can be performed at the main operating temperature. The product is factory-set to perform temperature control in the temperature control area.

When using the device, if the device does not properly control the temperature due to a rapid change in the operating environment (such as right after the purchase of the device or the reinstallation due to relocation) with respect to the user's main operating temperature, Auto Tuning can be done for accurate temperature control.

Auto Tuning temperature is performed by setting the target temperature value in the Basic Setting Mode and starting the control, then activate the Auto Tuning button to ON in System Setup> Auto Tuning.

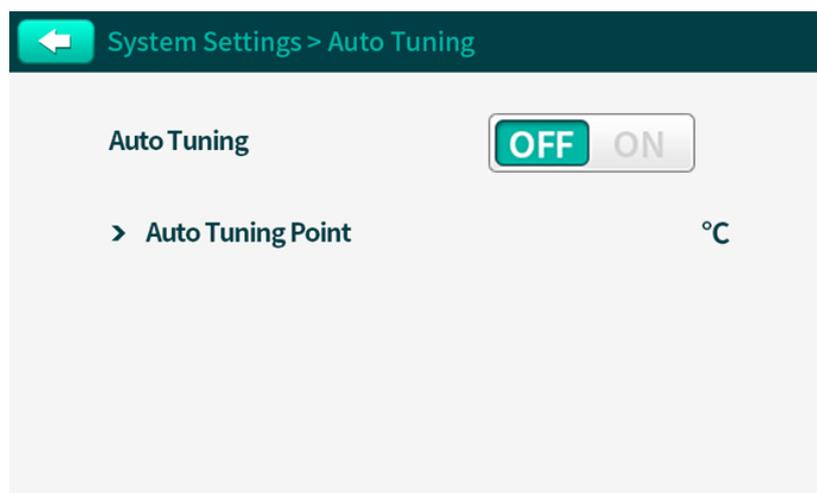

[How to set Auto Tuning]

- (1) After setting the temperature in Basic Mode, press the start button.
- (2) It is executed when the ON button is activated in the System Settings> Auto Tuning screen. The Auto Tuning function cannot be used when operation is stopped or in program control.
- (3) It moves directly to the operation display window of Basic Mode, and the icon  on the top status bar blinks indicating that Auto Tuning is running.
- (4) When Auto Tuning is completed, the icon  on the top status bar disappears and the Auto Tuning value is automatically saved.

NOTICE

- Auto Tuning may take tens of minutes or hours depending on the set temperature.
 - Do not turn off the power of the device while Auto Tuning is in progress.
 - During Auto Tuning, it is recommended that the difference from the ambient temperature be at least 30 degrees. If the Auto Tuning temperature is similar to the ambient temperature, the reliability of the optimal parameter value may be reduced.
 - Auto Tuning is not available when temperature control is stopped in Basic Mode or under temperature control in Program Mode.
-

4.5.4 Alarm


It is a function to generate an alarm when the temperature is above or below the user-specified temperature or when the door is opened [4.6.3 Refers to Alarm Display and Pop-up Notification Function].

The screenshot shows a mobile application interface for 'System Settings > Alarm'. It features four adjustable settings:

- High Deviation Temp.:** A plus sign followed by a text input field containing the value '5'.
- Low Deviation Temp.:** A minus sign followed by a text input field containing the value '5'.
- High Temperature:** A text input field containing the value '270'.
- Door Open Alarm Delay:** A text input field containing the value '5' followed by the unit 'min'.

Item	Function	Input Value	Default
High Deviation Temperature	Set the upper limit of temperature deviation. If the actual temperature becomes higher than the target temperature + allowable upper limit temperature, an alarm is generated.	0 ~ 250°C	5
Low Deviation Temperature	Set the lower limit of temperature deviation. If the actual temperature becomes lower than the target temperature - allowable lower limit temperature, an alarm is generated.	0 ~ 250°C	5
High Temperature	Set the absolute upper limit temperature. An alarm occurs if the actual temperature exceeds the absolute upper limit temperature.	0 ~ 270°C	270
Door Open Alarm Delay	Set the alarm for the door open delay time. If the door opens exceeding Door Open Alarm Delay, an alarm occurs.	Off (0) ~ 30min	5

4.5.5 Password

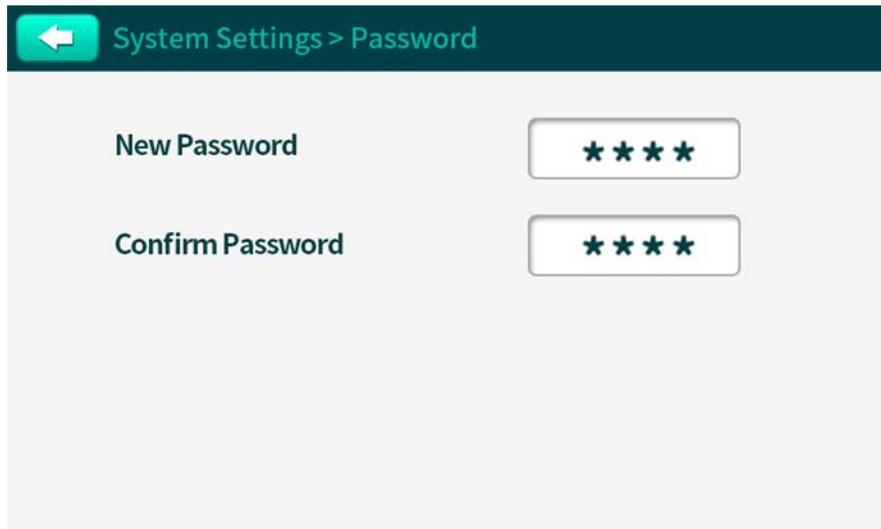


The initial value is set to '0000'.

Enter the desired password and press the back button  to complete the saving.

4.5.6 Factory Default

It is a function that initializes all values in the device at once.

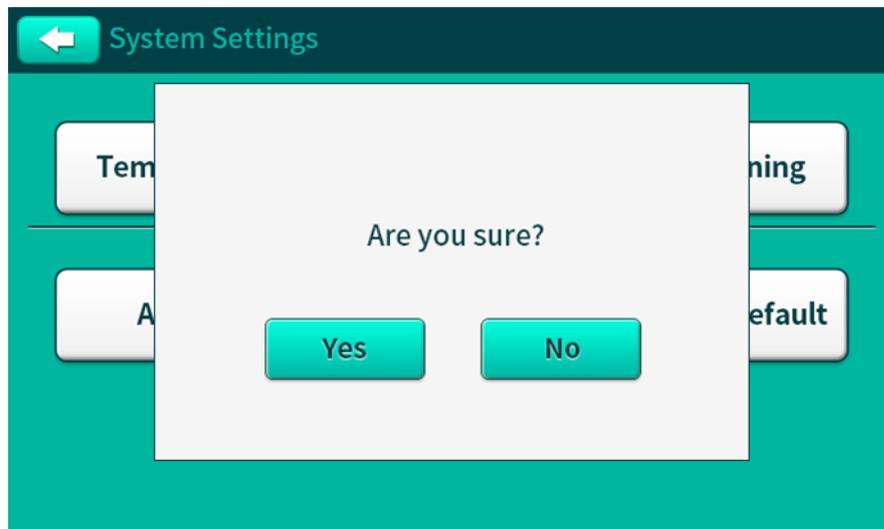

If you press the reset button, a pop-up notification appears and confirms whether or not to proceed with Factory Default.

This function initializes all settings changed in the Basic Settings, General Settings, and System Settings into the Factory Default values. When performing Factory Default, please be careful that all the values such as Auto Tuning and Temperature Calibration in the System Settings and General Settings are initialized.

4.6 Safety Function

4.6.1 Safety Functions Related to Temperature

(1) Temperature Limiter [4.7 Refer to Over temperature limiter]

If the temperature of the chamber rises abnormally above the set temperature (over 10~15% of SV) by using the electronic temperature limiter, an alarm sounds and the operation of the device stops.

4.6.2 Safety Functions Related to Use

(1) Door alarm

When the device operates with the door open, a beep sounds. Please close the door and try again.

If the door is opened while the device is operating, the heater stops and a warning message for door open appears. But there is no alarm sound. If the door is closed within the Door Open Alarm Delay time (default setting: 5 minutes), the previous operation continues. If the door is not closed after the entered time, a warning pop-up window appears with a beep. If a warning pop-up window is displayed, the device does not work even if the door is closed. In order to start the device again, close the door, check the warning pop-up window, and restart the machine. [4.5.4 Refer to Alarm for changing the Door Open Alarm Delay time]



(2) Touch Screen Lock Function

This button  is to turn on/off the lock function so that the touch screen cannot be used during the device operation.

(3) Circuit breaker

A circuit breaker is embedded to protect the device from short circuits or overcurrent.

4.6.3 Alarm Display and Pop-up Notification Function


This device provides Alarm Display function as shown in the table below for various states of the device.

In addition, if a problem occurs with the device during the system use, the following pop-up windows are provided to give information on problem solving. Check the notification message and please contact a service center referring to **9.4 Service Contact**.

Alarm Display Image	Contents
 High Temp. Deviation	Alarm displays when the actual temperature is higher than the target temperature + allowable upper limit temperature
 Low Temp. Deviation	Alarm displays when the actual temperature is lower than the target temperature – allowable lower limit temperature
 Temp. Rise Delay	Alarm displays when the temperature rise is delayed.
 High Temp.	Alarm displays when the temperature is over the absolute upper limit temperature that the device set
 Warning : Over Temp.	Alarm displays when the temperature of the device is higher than the temperature set in Over Temp Limit.
 Door : Opened	Alarm displays when the door is open.
 Door : Open time exceeded	Alarm displays when the door opens longer than the Door Open Alarm Delay time.
 Temp. Sensor Failure	Alarm displays when there is a problem with the temperature sensor.
 Board Failure	Alarm displays when there is a problem in the temperature detection circuit.

4.7 Over temperature limiter

Over Temperature Limiter is a device to prevent fire due to overheating. If the temperature of the heater rises abnormally above the temperature set in the Temperature Limiter, the temperature control is stopped and a warning window is displayed with a beep.

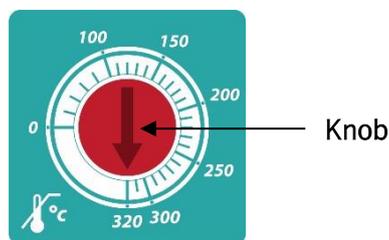

[Over temperature limiter]

※ If you want to use the Over Temperature Limiter as a temperature limiting function for sample protection, set it in the following order.

- (1) After setting the internal temperature of the instrument, press the Start/Stop button to operate the device.
- (2) When the target temperature is reached, the instrument should be stabilized for a certain period of time.
- (3) Turn the red knob counterclockwise using a screwdriver. Stop the knob when a warning is displayed on the screen with a notification sound.
- (4) Turn the red knob clockwise to set it at least 15% higher than the target temperature.

※ During temperature control, if the alarm sounds due to overheating, check the warning window and solve the cause of the problem. When the temperature goes down, it works again. If it is necessary to continue control with the same temperature, turn the red knob on the temperature limiter to set the temperature at least 15% higher than the set temperature, and press the Start button once to restart the unit.

5.0 Maintenance

5.1 Inspection Cycle

Category	Inspection Timetable				
	Daily	Weekly	Daily	Quarterly	Daily
General Checklist					
Power Cord					
Check the instrument and the power connection	•				
Check the damage of the power cord	•				
Cleanness of external part		•			
Cleanness of internal part		•			
Cleanness of accessories		•			
System (Control) Related Checklist					
Check clock accuracy		•			
Automatic tuning				•	
Temperature calibration					
Check the temperature offset value					•
Calibrating actual temperature/ displaying temperature					•
Check temperature setting value	•				
Check temperature limiter operation	•				
Check function of controller				•	
Electric wire related checklist					
Defects if electric wire			•		
Check contamination of electric wire			•		
Check fixation of wiring fasteners			•		

⚠ CAUTION

- Before using the instrument, please check if there is any other foreign material inside the chamber, and keep it clean.
 - Be careful not to damage accessories or systems inside the instrument.
 - Be careful not to contact the main body with high concentrations of nitric acid, sulfuric acid, sodium hydroxide or corrosive solvents such as acetone, benzene, phenol, toluene, chloroform, crezol, acetic acid, chloroform.
-

⚠ WARNING

- Check the general, system(control), and electric wire related checklist according to the inspection cycle.
 - If the inspection cycle are not followed, the manufacturer is not liable for any damage to the equipment or fire that may occur.
-

5.2 Cleaning the Instrument

To keep the instrument in the best condition, to operate it effectively, and to extend its life, it has to be cleaned regularly. It is recommended to check the cleanness daily, clean the internal part weekly, and clean the exterior part monthly.



WARNING

- If the instrument is contaminated from special use, please wipe immediately.
- Since there is a risk of electric shock, please make sure to turn off the power switch and disconnect the plug from the outlet. Also, please wear chemical-resistant gloves.

Please follow the guidelines as shown below.

5.2.1 Cleaning the interior part of the instrument

(1) In general

Step 1: Take out the shelf from the instrument and wipe it with a dry cloth using a neutral detergent.

Step 2: Wipe the inner surface of the instrument with a dry cloth using a neutral detergent.

(2) In case of contaminated

If the device is contaminated with toxic chemicals or toxic gases, please clean it according to the following guidelines.

Step 1: Make sure to wear chemical-resistant gloves and masks.

Step 2: Wipe the contaminated parts of the instrument with a dry cloth.

Step 3: Wipe it with a soft cloth or sponge using a neutral detergent, and then wipe again with a dry cloth.

5.2.2 Cleaning exterior part of the instrument

Step 1: Wipe the exterior surface of the device using a wet soft cloth. If the contamination is severe, wipe with a soft cloth or sponge using a neutral detergent.

Step 2: Wipe it again with a dry cloth.

5.2.3 Cleaning the accessories

Wipe the accessories with a soft cloth or sponge using a neutral detergent, and then with a dry cloth.

⚠ CAUTION

- Since there is a risk of electric shock, before cleaning, please turn off the power switch and disconnect the plug from the outlet.
 - If the device is contaminated with toxic chemicals or gases, please make sure to wear chemical-resistant gloves and masks when cleaning the interior part.
 - Never use chlorine detergent. It may cause the chamber to be oxidized. Also, never use volatile substances such as cleaning agents, abrasives, benzene, acids or solvents.
 - Do not wipe the surface of the instrument using an organic solvent such as sulfuric acid or hydrochloric acid.
 - Use a soft cloth or a sponge to wash the cleaning tool with a neutral detergent.
 - Do not pour water directly into the instrument while cleaning.
 - Do not arbitrarily disassemble and clean the instrument.
 - If cleaning the instrument in a way other than the above method, please check with JEIOTECH or the branch before cleaning.
-

5.3 Major maintenance checks

Please check the confirmation below once again and operate the device correctly.

- (1) Please check the connection between the device and the power source.
- (2) Please check whether the device and system are correctly fixed in the caster.
- (3) Please check whether the up/down, left/right horizontality of the device is correct.
- (4) Please check if there are any flammable or explosive substances left in the device.



WARNING

- Do not arbitrarily disassemble or modify the device other than what is described in this user manual.
 - When handling electrical components inside the device, it must be handled only by qualified people.
-

5.4 Movement and storage

- (1) When moving the instrument, remove the power plug from the outlet.
- (2) Take out everything from the inside of the instrument.
- (3) Before moving the instrument, close the door completely.
- (4) Do not move the instrument by holding the door of the instrument.
- (5) Please pack the equipment, part, and accessories in their original packaging or use appropriate packaging to protect the product during transportation.
- (6) When the instrument is not in use for a long period of time, unplug the power plug, clean it, pack it, and store it in a dry place.



WARNING

- Do not move the instrument with the power cord connected.
 - Do not move the instrument while it is in operation.
-



CAUTION

- Be careful when transporting the instrument since it is heavy. Use the appropriate required tools for transport, and carry it two or more people together.
 - Do not move the instrument while holding the door.
 - Do not cause mechanical shock or vibration during movement or storage of the instrument. Internal damage may cause problems with operation.
 - Disconnect the power plug when the instrument is not in use.
-

6.0 Trouble Shooting

6.1 Trouble Shootings for abnormalities

If an abnormality occurs while using the instrument, please check the following according to the guidelines. If you can't solve the problem even if you check the following or not presented problems, please immediately request the technical service to JEIOTECH's sales department. If the device is not operating, please check the followings.

(1) Please check the power connected to the instrument.

(2) Please check if the START button is pressed.

(3) Please make sure there is no power outage.

6.2 Power Trouble Shootings for abnormalities

Problem	Cause	Solution
The device does not turn on or has turned off while in use.	<ul style="list-style-type: none"> The power cord is not connected to the outlet correctly. 	<ul style="list-style-type: none"> Plug the power cord into the outlet correctly.
	<ul style="list-style-type: none"> Outlet/ plug/ power cord is damaged. 	<ul style="list-style-type: none"> Replace the damaged outlet/ plug/ power cord.
	<ul style="list-style-type: none"> Power supply does not match the equipment's power type. 	<ul style="list-style-type: none"> Check the voltage, phase and capacity of the power supply and connect the power correctly.
	<ul style="list-style-type: none"> Either circuit breaker is tripped or there is a power outage. 	<ul style="list-style-type: none"> If the electrical circuit breaker in the building is tripped, find the cause of the short circuit and fix it.
	<ul style="list-style-type: none"> Internal circuit failure of the equipment 	<ul style="list-style-type: none"> Request service.
Circuit breaker in the building keeps tripped.	<ul style="list-style-type: none"> Too many plugs are connected. 	<ul style="list-style-type: none"> Remove all the devices connected to the circuit breaker and use within the capacity of the circuit breaker current.
	<ul style="list-style-type: none"> Internal circuit failure of the equipment 	<ul style="list-style-type: none"> Request service.
The power turns on but the equipment does not work.	<ul style="list-style-type: none"> Due to overheating, the protection device cuts off the power. 	<ul style="list-style-type: none"> When the internal circuit board is overheated, the device automatically shuts off the heater power to protect the internal circuit and emits alarm. Unplug the power cord and allow the equipment cool, then restart.
	<ul style="list-style-type: none"> Internal circuit failure of the equipment 	<ul style="list-style-type: none"> Request service.

6.3 Error Handlings

Problem	Cause	Solution
In case the alarm keep ringing	• Door is opened	• Please check if the door-opened lamp is working, and then close the door.
	• The setting temperature Over temp. limiter is abnormal	• Set the 15% higher temperature of the Over temp. limiter.
In case the temperature does not rise	• Check if the "Run" sign of the status display is blinking (placed on the top part of the controller)	• Press the "Start/Stop" button if the "Run" sign is turned off.
	• Door is opened	• Close the door.
	• Door switch failure	• Open and close the door 2-3 times to check for any abnormality in the door switch. • Request for the technical service.
	• The set set temperature is lower than the current temperature.	• Check the set temperature and enter the temperature you want to use.
	• Timer setting	• Check the Wait on timer
	• Device failure	• Request service.
In case the temperature control is not working	• Please check whether there is any device that generates strong high frequency noise around the instrument.	Please remove such devices that generate strong high frequency noise.
	• Did not perform Auto tuning	• Execute the Auto tuning
	• Foreign substances or oil may be introduced into the controller	• Request for the technical service.
	• Device failure	• Request service.
In case the abnormal sound	• Fan Failure	• Check if the fan is working normally. • Request for the technical service.
	• Device failure	• Request service.
In case the display is abnormal	• Damage to parts due to external force, chemicals, or overheating	• Request service.
In case the touch does not work well	• Touch with a large area such as your finger or touch with low pressure	• The display of this device is piezoelectric, so touch it with a hard part of your hand, such as your fingernail.

※ If parts are needed to be replaced, only pure parts should be used.

※ Failure beyond normal limits cannot maintain technical repair.

6.4 Caution and warning alarms

The equipment provides an alarm display function as shown in the table below for Caution and warning. In addition, troubleshooting information is provided in a pop-up window when an error occurs for the convenience of users while using the equipment. Check the message and take action referring to [9.4 Contact Points].

6.4.1 Caution

Problem	Cause	Solution
 High Temp. Deviation	the actual temperature is higher than the set temperature + allowable upper limit temperature	Stop the instrument and restart it after the instrument has cooled down. If the same problem occurs, request service.
 Low Temp. Deviation	the actual temperature is lower than the set temperature – allowable lower limit temperature	Stop the instrument and restart it after the instrument has cooled down. If the same problem occurs, request service.
 Door : Opened	door is open	Check if the door text on the display window is on and close the door securely.
 Temp. Rise Delay	The temperature rise is delayed.	Please check the operating environment.

6.4.2 Warning

Problem	Cause	Solution
 High Temp.	the temperature is over the absolute upper limit temperature that the device set	Unplug the power cord and restart the device after it cools down.
 Warning : Over Temp.	The temperature of the device is higher than the temperature set in Over Temp Limit.	Set the over temp limiter 15% higher than the current temperature. (Set up to a maximum temperature of 270 degrees)
 Door : Open time exceeded	The door opens longer than the Door Open Alarm Delay time.	Close the door and start the instrument or change the door open delay time setting.
 Temp. Sensor Failure	There is a problem with the temperature sensor.	Request service.
 Board Failure	There is a problem in the temperature detection circuit.	Request service.

7.0 Accessories

7.1 Types of Accessories

Designation		Cat. No.	Description
Wire shelf	OF4-03	FDA0009739	-
	OF4-05	FDA0009738	-
	OF4-10	FDA0009737	-
	OF4-15	FDA0009736	-
Perforated shelf	OF4-03	AAA125341	(Option)
	OF4-05	AAA125342	(Option)
	OF4-10	AAA125343	(Option)
	OF4-15	AAA125344	(Option)
Stacking Set	OF4/ON4/IB4-A/IB4-05	AAA125547	(Option)
	OF4/ON4/IB4-A/IB4-15	AAA125549	(Option)
BMS port, Connector	OF/ON4_03,05,10,15	AAA125534	(Option)

CAUTION

- Ovens or incubators of the same size using a Stacking Set can greatly increase laboratory space efficiency. However, the minimum control temperature of the upper chamber may be limited due to the heat generated by the lower chamber as shown below.
 1. When placing the oven at the bottom and the incubator at the top: Depending on the oven's set temperature, the minimum control temperature of the incubator can increase by up to amb+25°C.
 2. When placing ovens at both the top and bottom: The temperature range of the upper oven can increase by up to amb+25°C, depending on the set temperature of the lower oven.
- Therefore, to ensure the minimum control temperature of the upper product, it is recommended to use the lower product at a low temperature and the upper product at a high temperature.

7.2 LC Green Box (Option)

This device connects JEIOTECH laboratory research equipment into one network, enabling an experimenter to operate the equipment more efficiently.

After connecting the equipment to LC GreenBox, you can use the LC Connected service, which enables mobile mentoring and control of the equipment's current operating status and faults.

(You can connect up to four devices to one LC GreenBox.)



Item	Cat. No.	Dimension (W x D x H, mm)	Figure
LC GreenBox	AAAQ1011	156 x 94 x 100 (with antenna)	


8.0 Dedicated Software

8.1 Installing the Monitoring Program


You can go to the site address below and download the JeioTechSoft program from support → software.

<https://www.jeiotech.com/>.


- (1) After downloading the application program, click “Next” to change the screen to License agreement.

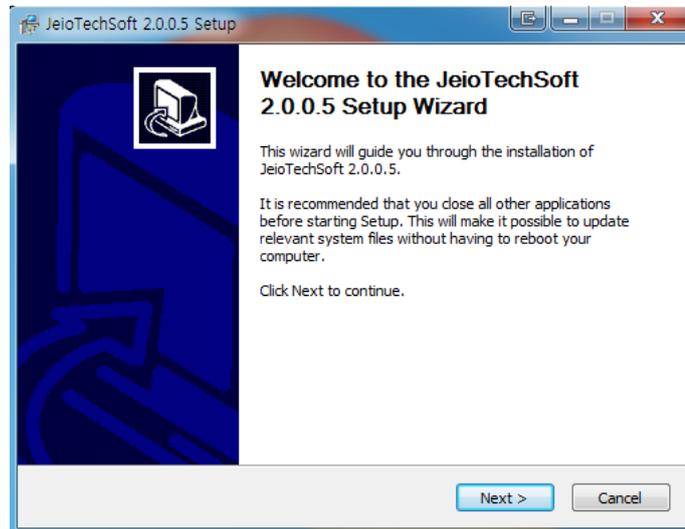

- (2) If you reviewed all the License contents, press “I agree” to install JeioTechSoft.

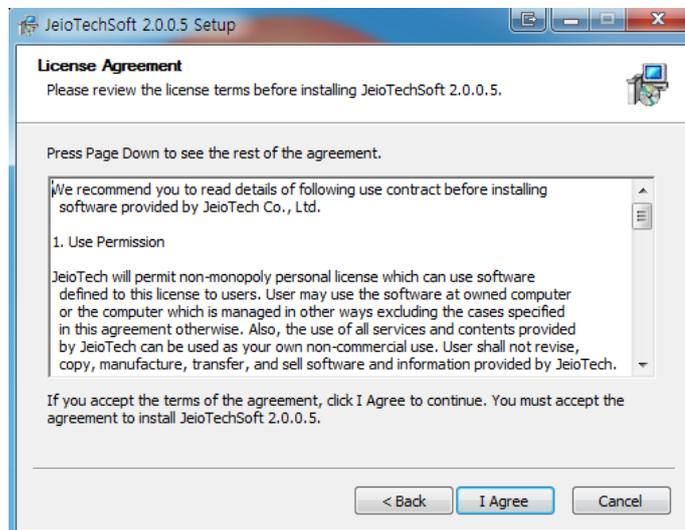


- (3) Press “Install” to start the program installation after specifying the saving path.

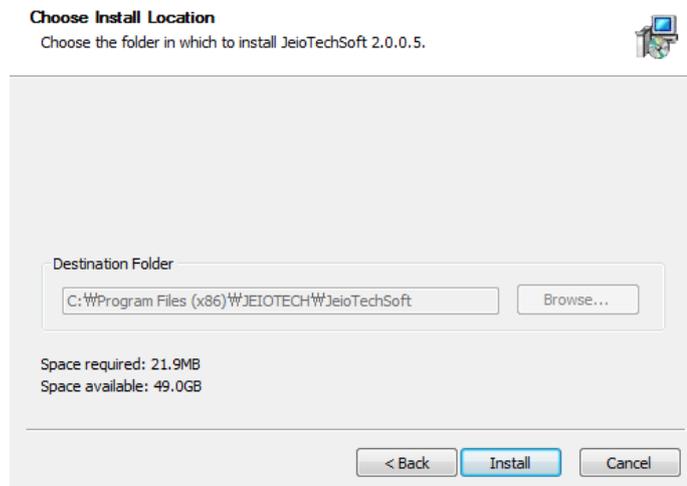


- (4) When the program installation is completed, the JeioTechSoft icon will be created on the desktop. Please launch the program by checking the JeioTechSoft 2.0.0.5 list box or double-clicking the icon on your desktop.

8.2 Connecting the software to the instrument

- (1) Run the dedicated software, “JeioTechSoft.”
(2) Press the connection button to start.

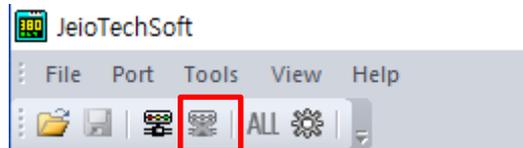


- (3) If the “Connection” window pops up, please check the appropriate device number for PORT and enter the same number as PORT in the General Settings > Communication Device Number. (Please check the communication port and the instrument number in the computer. Control Panel > Device and Printer > Device Manager > Ports (COM & LPT)).

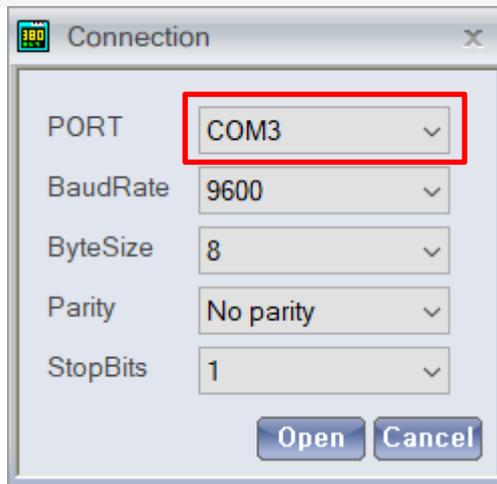

* The initial values of the "Connection" window

PORT	Baud Rate	Byte Size	Parity	StopBits
COM1	9600	8	No parity	1

- (4) Please match the instrument number and the value of the "Connection" window. Click Open to link the instrument and computer.

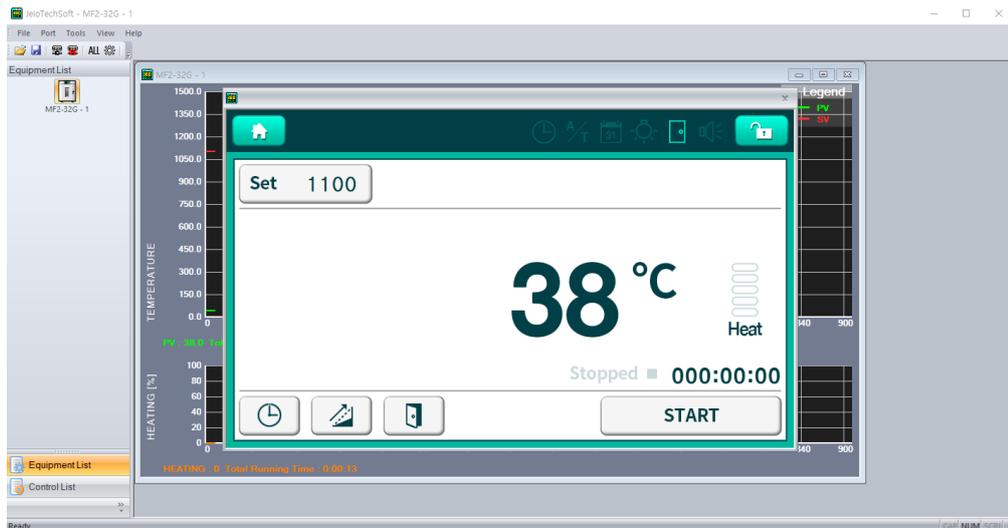

NOTICE

- When running the JeioTechSoft program via the communication port, the input values of the temperature, timer, and pump circulation can be entered directly by the numeric keypad on the computer keyboard or by the \uparrow or \downarrow of the direction keys. At this point, the number of digits of the input value can be moved by using the \leftarrow or \rightarrow directional keys, or by entering "." at the decimal place.
- Press the Delete key on your computer keyboard to set the input value to "0".
- If you enter a value that is greater than the inputable value, the maximum inputable value will be entered.

8.3 Communication Protocol

8.3.1 Overview of Communication Protocol

Communication Speed: 9600, 19200, 57600 bps

Parity: none, Odd, Even

Protocol: MODBUS-RTU

Communication Address: 0 (Broad Casting), 1~255

8.3.2 Data Format

Contents	RTU
Header	None
Trailer	None
Data length	8-bit (fixed)
Data format	Binary
Error detection	CRC-16 (Polynomial = 0xA001)
Data time interval	Less than 24-bit

8.3.3 Frame

Header	Communication Address	Function Code	Data	CRC Check	Trailer
None	8-bit	8-bit	n * 8-bit	16-bit	None

8.3.4 Function Code

The MODBUS communication function code consists of a function code that can read/write the contents of the D-Register and a loop-back detection function code.

Function Code	Contents
03	D-Register Continuous Read
06	Single D-Register Write
08	Diagnostics (Loop-Back Test)
16	D-Register Continuous Write

The time that MODBUS RTU recognizes as the start of communication is "3.5 Character" + "maximum 2ms".

Please visit the www.jeiotech.com site and download the JeioTechSoft program from support → software.

9.0 Appendix

9.1 Technical Specification

9.1.1 OF4-P Series

Item/Model		OF4-03P(W)	OF4-05P(W)	OF4-10P(W)	OF4-15P(W)
Chamber volume (L/cu ft)		26/0.92	61/2.15	112/3.96	147/5.19
Temp.	Range (°C/°F)	Amb. +10 ~ 250/18~482			
	Fluctuation at 100°C (°C/°F)	±0.3/0.54	±0.3/0.54	±0.3/0.54	±0.3/0.54
	Variation at 100°C (°C/°F)	±1.4/2.52	±1.9/3.42	±1.7/3.06	±1.5/2.7
	Heating time to 100°C (min.)	8	10	14	15
	Recovery time at 100°C (min.)	4	4	4	4
	Controller	Microprocessor PID			
	Sensor	PT 100			
	Heater (SUS 304, 230VAC/120VAC, W)	1400			
Controller functions		Auto tuning, 3-point temp. calibration, Wait on / off timer(99hr 59min), Auto-run			
Safety		CLS(Custom Logical Safe)-control system, IEC protection Class I, Over temp. limit			
Control panel		5inch TFT Color LCD			
Communication interface		USB, RS-232 BMS (Option)			
Material	Internal	Stainless steel			
	External	Steel, 0.8t powder coating			
	Shelves	Stainless steel wire, electro polished			
	Insulation	Mineral wool			
	Viewing window(Optional)	Tempered safety glass, two fold, 5t			
	Ventilation slide	Stainless steel, dia 38mm x 1ea			
Dimensions	Interior (W x D x H, mm/inch)	300x210x400/ 11.8x8.27x15.75	380x330x480/ 14.97x13.0x18.9	485x350x655/ 19.1x13.78x25.79	550x376x710/ 21.65x14.8x28.0
	Exterior (W x D x H, mm/inch)	478x527x604/ 18.8x20.75x23.78	558x648x684/ 21.97x25.5x26.93	663x677x859/ 26.1x26.65x33.82	728x704x914/ 28.66x27.7x36.0
	Shelves (standard / max)	2/4	2/5	2/8	2/9
	Glass door (W x H, mm/inch)	264 x 260, 5t/ 10.39x10.23, 0.2t	300 x 270, 5t/ 11.81x10.63, 0.2t	423 x 330, 5t/ 16.65x12.99, 0.2t	423 x 330, 5t/ 16.65x12.99, 0.2t
Electric requirements (VAC, Hz, A)		230, 50/60, 6.4 120, 60, 12.3			
Electric consumption (Wh)		40 (at 100°C) 790 (at 250°C)	60 (at 100°C) 810 (at 250°C)	70 (at 100°C) 1090 (at 250°C)	80 (at 100°C) 1240 (at 250°C)
Max. load per shelf (kg/lbs)		20/44.09			
Noise Level (dB)		48			
Number of Air change per hour at 100°C		123	22	18	11
Weight (net, kg/lbs)		33/72.8	53/116.8	63/138.9	73/160.9
Permissible ambient temperature (°C/°F)		5 - 40/41-104			
Permissible relative humidity (%)		10 - 80			

※ The above specifications are subject to change without individual notice due to product quality and performance improvement.

※ CE Models: 230 VAC, 50/60 Hz models fulfill the requirements of relevant European product directives

9.2 Disposal of Product

Before disposing a product or its component, please be aware of the followings.



- (1) This product is potentially hazardous when exposed to biological, chemical, or radioactive materials, so it must be cleaned up to protect disposal personnel, waste collectors, and the environment.
- (2) Please contact a person in charge of disposing of the products to check the electrical, electronic, and material disposal standards. When you request externally, it is recommended that you contact your company's vendor or a testing equipment manufacturer that can properly dispose of the laboratory equipment and its components.

9.3 Warranty

9.3.1 Warranty period

- (1) If the product fails during normal and proper use, the warranty period for manufacturing liability shall be two years from the date of delivery.
- (2) If you request a repair, please check the items below and let us know so that you can get a quicker and more accurate repair.

- | |
|---|
| <ul style="list-style-type: none">• Date of purchase:• Customer name / address / phone number / E-mail:• Fault status• Model• Serial number |
|---|

9.3.2 Technical Service Contact Points

Technical Services

Address : 153 (Youngsan-dong), Techno 2-ro Yuseong-gu, Daejeon-city, 34025, Republic of Korea

Tel : +82 (0)2 -2627-3824

Website : <https://www.jeiotech.com/eng/>

E-mail : overseas@jeiotech.com

9.3.3 Certificate of Product Warranty

This is a guide to the product quality warranty and service terms provided by JEIOTECH Co., Ltd

All products are guaranteed to operate normally when installed under proper conditions, as specified in the user manual for each product, and used according to the intended purposes and permissible operating conditions.

The warranty period for product quality starts from the delivery date and is indicated in the catalog provided for each product or in the purchase order agreed upon with the customer. If a product malfunctions within the warranty period, JEIOTECH Co., Ltd. provides free repair services. However, among the transportation costs incurred during the repair process, any special costs resulting from the customer's site conditions (e.g., door or wall modifications, use of special handling equipment) are not covered under the warranty. Furthermore, JEIOTECH's liability under this warranty is limited to replacing the product or refunding the original purchase price at JEIOTECH's sole discretion if reasonable attempts to repair or replace the product fail.

Parts replaced during free repairs within the warranty period become the property of JEIOTECH Co., Ltd. Additionally, the warranty period is not extended due to free repairs. JEIOTECH is not responsible for any losses incurred by the customer due to delays in repairs caused by issues such as part shortages or shipping delays.

The following cases will be handled as paid repairs, even within the warranty period:

1. Non-defective cases

- * Requests to resolve issues arising from improper operating environments or abnormal installations.
- * Reinstallation requests or connections with external equipment other than the initial installation.
- * Requests for usage instructions or simple adjustments that do not require disassembly.
- * Inspections of non-defective products.
- * Cleaning or debris removal service requests.

2. Failures caused by user errors:

- * Malfunctions due to usage not in accordance with the user manual.
- * Issues resulting from improper operating environments or abnormal installations.
- * Malfunctions caused by incompatible chemical usage.
- * Malfunctions caused by irregular or improper electrical or utility supplies.
- * Damage due to product movement, storage, external impact, or dropping by the customer.
- * Malfunctions resulting from unauthorized modifications or repairs without prior written approval from JEIOTECH Co., Ltd.
- * Malfunctions caused by using consumables or optional components not specified by JEIOTECH Co., Ltd.

Ltd.

- * Repairs performed by personnel other than JEIOTECH or its authorized service agents.

3. Other cases

- * When the product model or serial number has been damaged, removed, manipulated, or altered.
- * Malfunctions caused by fire, flooding, or other natural disasters.
- * Failure due to consumable parts reaching the end of their lifespan (e.g., lamps, filters, fuses, gaskets, packings, hoses, heat transfer fluids).
- * Natural wear and tear (e.g., discoloration, screen printing degradation).
- * Damage or malfunction of product accessories (e.g., power cables, data cables, glass components) or options.
- * Malfunctions caused by errors in computers, computer components, or connected network systems.

- Before JEIOTECH performs free or paid repairs or accepts the return of a product, the customer must ensure the product has been decontaminated of chemical and biological hazards.
- Replacement parts used during repairs may differ from the original but will function correctly and be equivalent in performance.

- JEIOTECH does not bear any responsibility for damage to stored samples, data loss, or any other direct or indirect damages caused by product malfunctions, regardless of the warranty period.
- JEIOTECH does not guarantee issues related to computers, computer components, or network systems connected to the product, regardless of the warranty period.
- This warranty is the sole and exclusive warranty provided. Any implied warranties imposed by applicable laws are limited to the warranty period stated herein. This warranty cannot be modified by any verbal advice, statements, or documents on behalf of JEIOTECH unless explicitly labeled as a "Warranty Amendment" and signed by an authorized representative of JEIOTECH.
- This warranty applies only to products purchased for direct use by the customer. It does not cover products purchased for resale purposes without prior written approval from JEIOTECH.
- This warranty does not apply to consumables and is non-transferable.

- The contents of this manual are subject to change without notice to improve the performance of the product and to ensure accurate information delivery.
- Copyright of this manual is in JEIOTECH.